

PROCESS NMR ASSOCIATES


# **Bench-Top and On-Line High Resolution Permanent Magnet 60 MHz NMR For Reaction Monitoring and Process Control**

**Presented By**

**John Edwards, Ph.D.**

**Process NMR Associates, LLC  
Danbury, Connecticut**

**January 25, 2011  
ABQMR/NMR, Albuquerque, NM**



# PROCESS NMR ASSOCIATES

250+ Analytical NMR Customers

smiths detection  
bringing technology to life





MODCON



QUALION  
NMR ANALYZERS



Swagelok

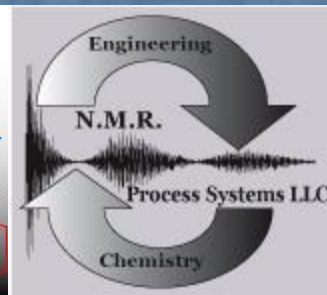

TTC Labs, Inc.  
*Process Engineering Excellence*




TopNIR Systems



RESONANCE  
SYSTEMS






PROCESS NMR ASSOCIATES

## High Resolution FT-NMR – Online / in Process









PROCESS NMR ASSOCIATES

## NMR Sample System and Placement

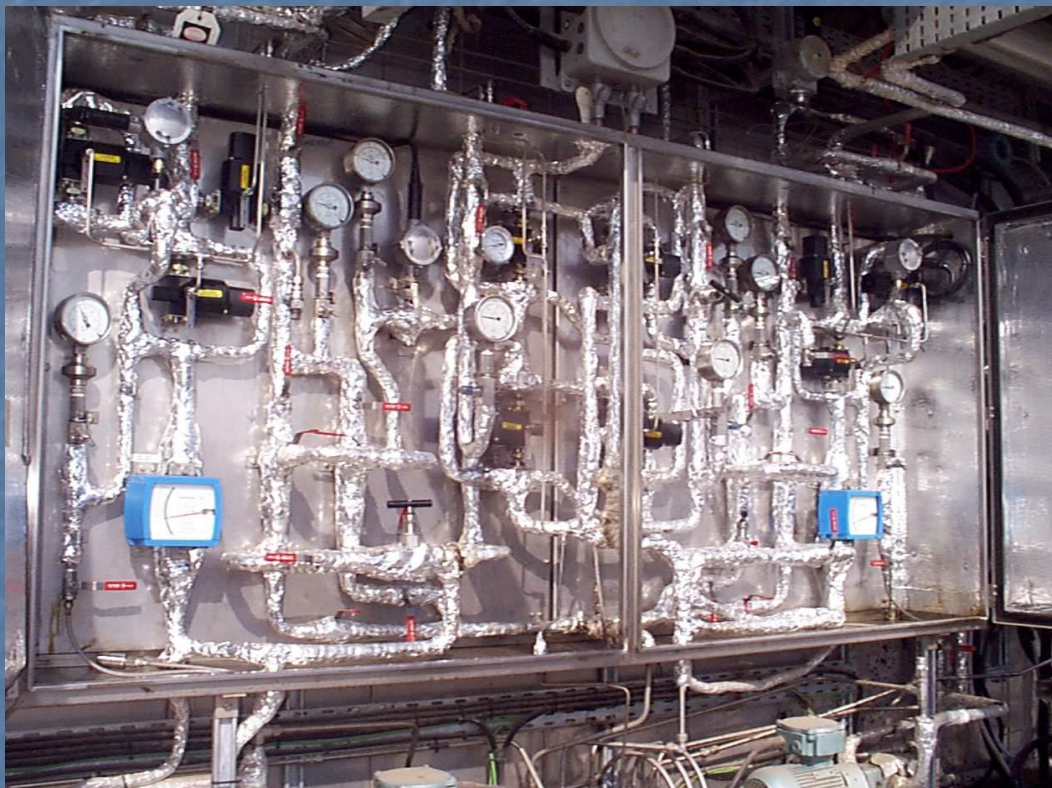




PROCESS NMR ASSOCIATES

NMR Lock - External  $^7\text{Li}$  Lock @ 22.5 MHz    Shim DACs Built into the Magnet Enclosure



Matrix Shimming Performed  
by Optimizing FID RMS






# PROCESS NMR ASSOCIATES



## SPECIFICATIONS


<b>Nuclei Observed</b>	H <sup>+</sup> (primary)
<b>Operating Frequency</b>	58±1.0 MHz for H <sup>+</sup>
<b>Sample Tube</b>	Standard laboratory glass tube L: 35.5 cm O.D 8 mm - I.D 7 mm Other size optional
<b>Sample Temperature Heating</b>	Controlled between 30°C – 80°C (86°F to 176°F)
<b>Magnet System</b>	Temperature stabilized, self-condensed field, permanent (neodymium) magnet with integral field gradient (shim) coils and automatic shim control
<b>Field Strength</b>	1.35 Tesla at 45°C
<b>Fringe Field</b>	Less than 1 gauss on external enclosure of magnet
<b>Dimensions</b>	145 cm H x 106 cm W x 65 cm D (57 in H x 42 in W x 26 in D) Add 15 cm (6 in) to height for shipping pallet
<b>Enclosure</b>	Self standing, wheel driven carriage
<b>Weight</b>	400 kg (882 lb) net weight 444 kg (980 lb) gross shipping weight
<b>Power Requirement</b>	220-240 Vac, 3500W maximum 110-120 Vac, 3500W maximum
<b>Other Utilities</b>	Internal Air condition system for higher stability
<b>Operating temperature</b>	Ambient Range: Temperature controlled environment
<b>Relative humidity</b>	Min / Max 30%-50%.
<b>Vibration</b>	Max: 0.3 mm/s <sup>2</sup> on the 3 axes
<b>Communication</b>	Local Ethernet Base -10/100. Remote connection via modem.





# PROCESS NMR ASSOCIATES





**New magnet design solves the problem of:**

Long term and short term Stability  
Temperature sensitivity

# New Magnet System

**State of the Art electronics:**



Smaller foot-print  
40 Shim coils on 2 single PCB  
Integrated PCB for Shim & Heater Control  
Digital RF & Acquisition –  
improve SNR

**New concept of Process Probe:**

Entire sample pipe through  
without contact with the system  
Much better temperature  
insulation  
Higher Q (better sensitivity)


**New Software:**

Includes new algorithm for  
standard and global Models  
Fully automated process capacity  
Extensive remote diagnostic capabilities

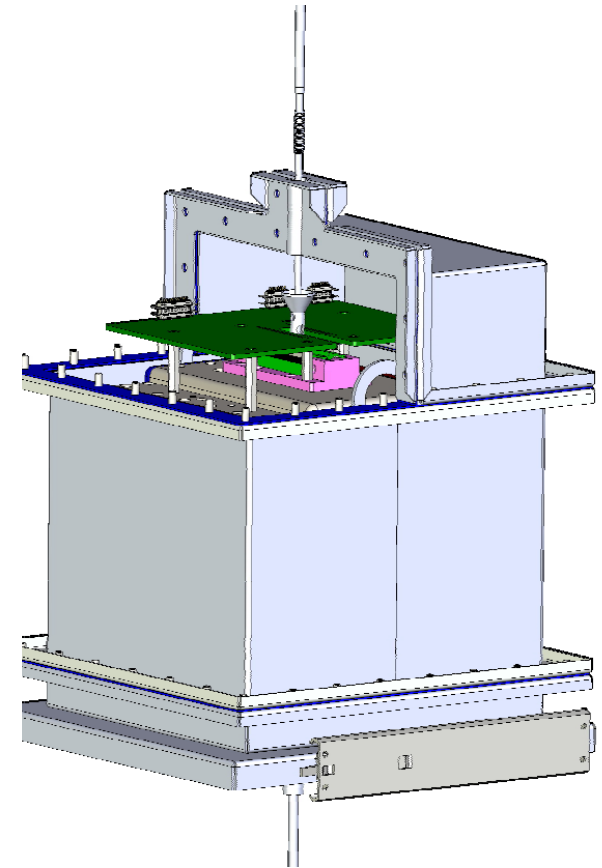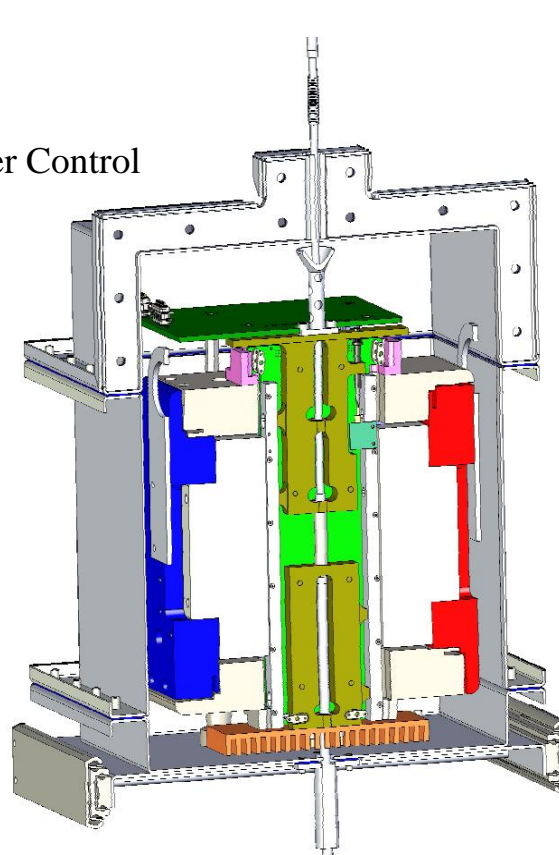





17-22 kg – 15 mm clear bore – 71 MHz  
6 mm homogenous zone (Magenta Line is  $\pm 0.1$  ppm)

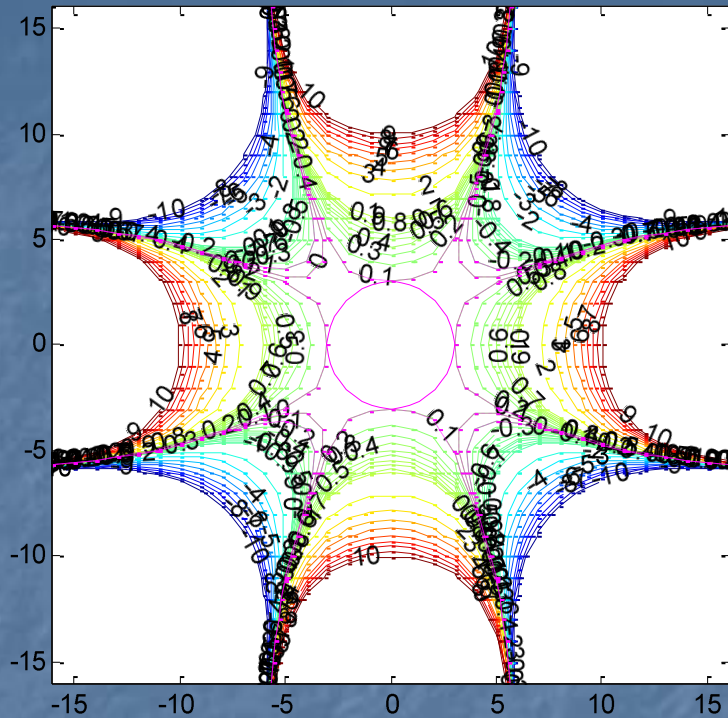

Plane parallel in the magnet center to the poles

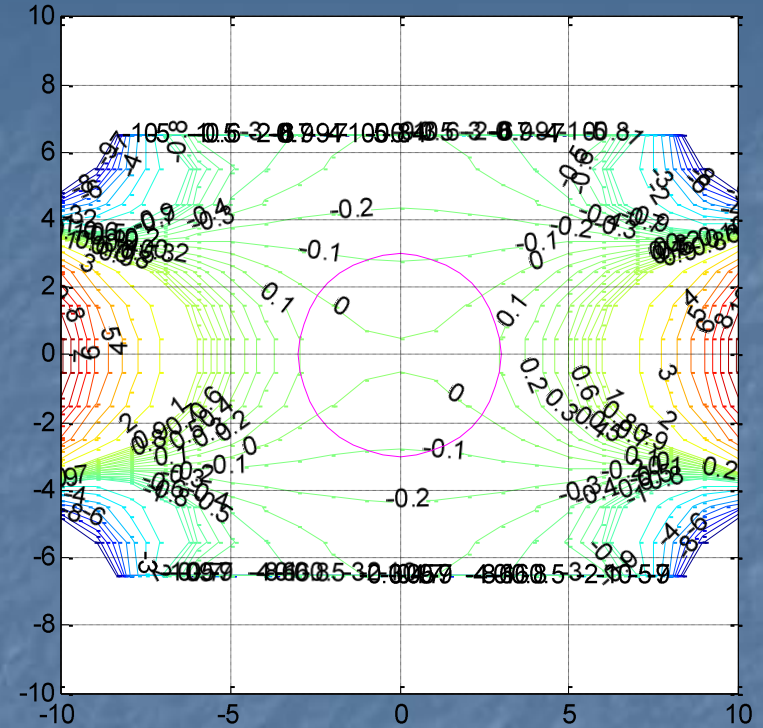


Plane perpendicular to the pole in the magnet center

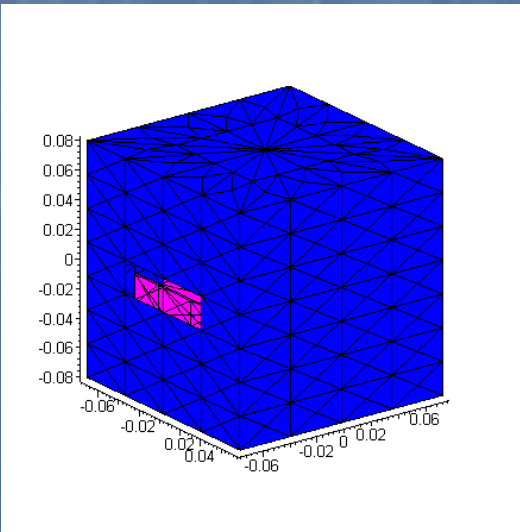

Magnet Dimension in Meters  
(14x14x17cm)

Calculation based on requirement  
Of 5 mm sample tube.








# PROCESS NMR ASSOCIATES


FT- $^{13}\text{C}$

FT- $^1\text{H}$

300 MHz


58 MHz

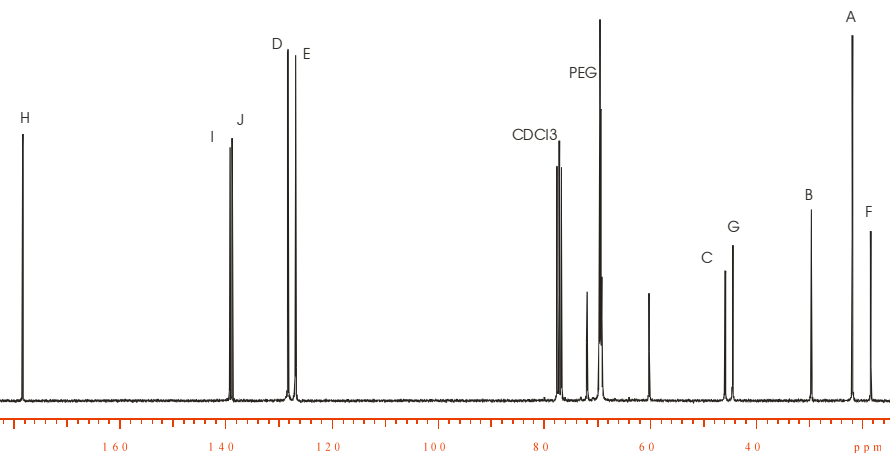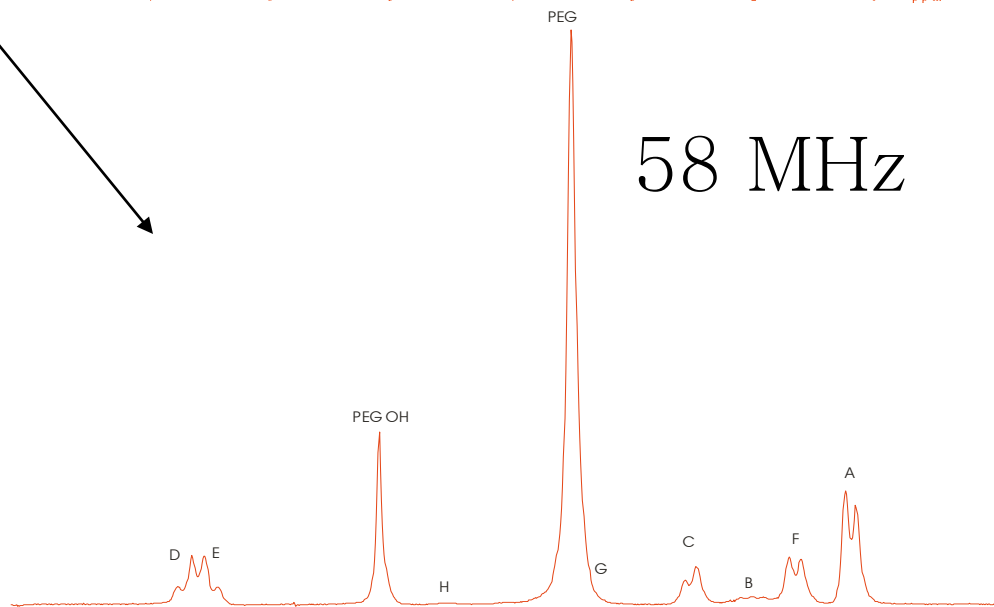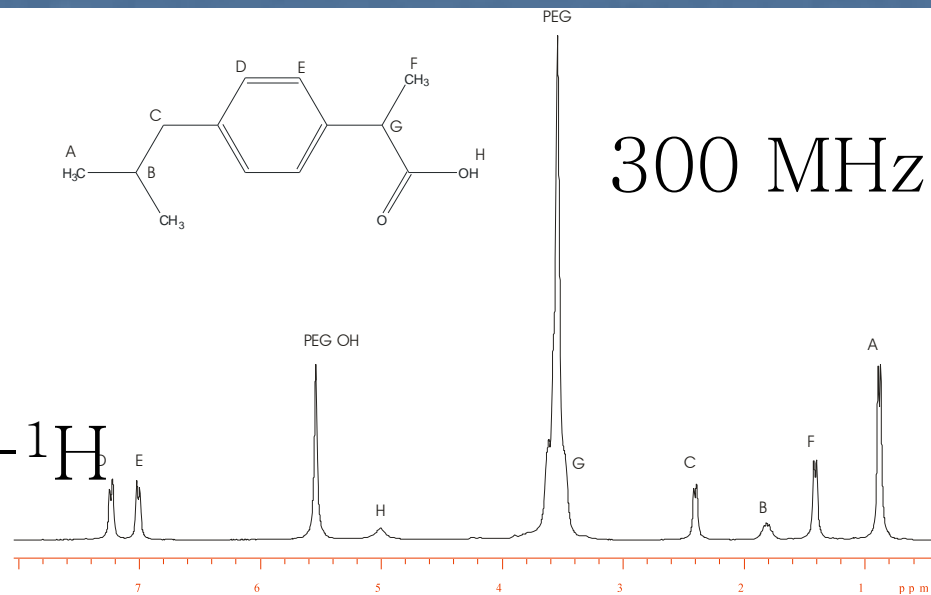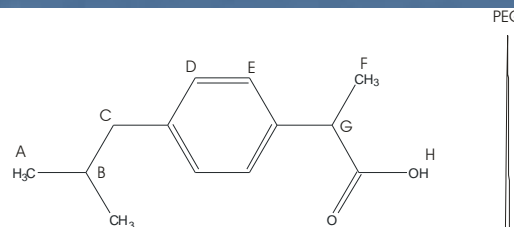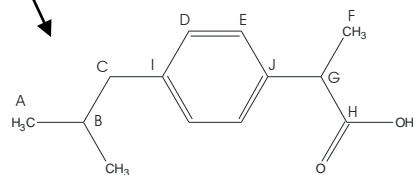

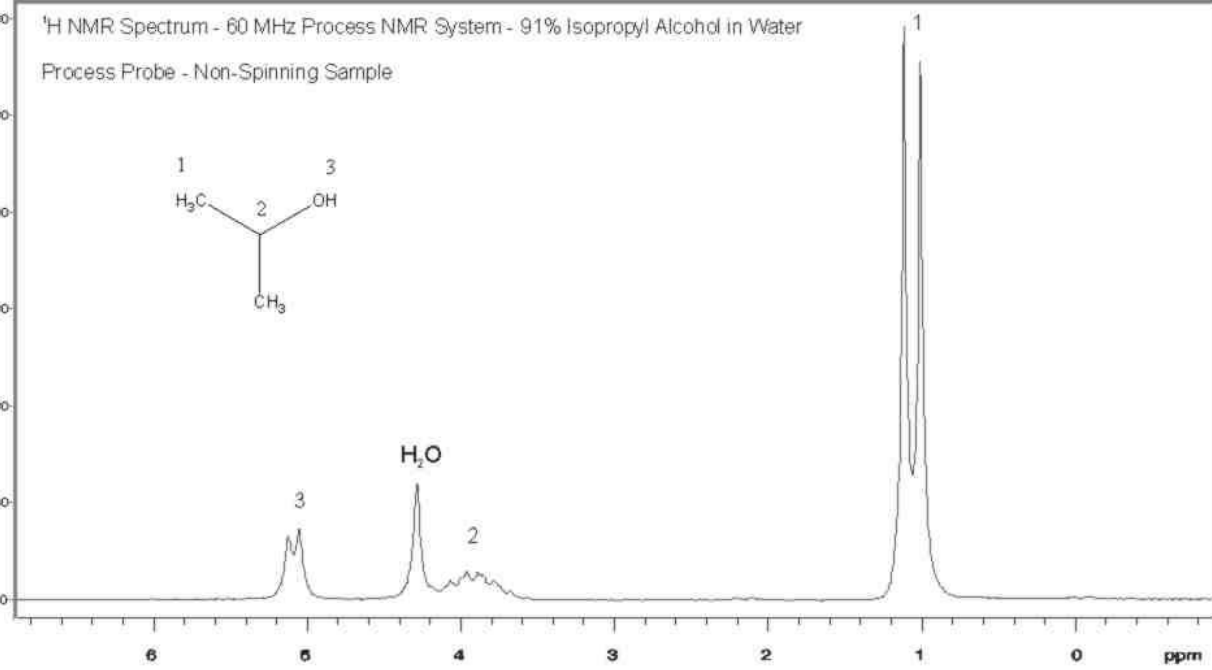




Arbitrary / Arbitrary  
File # 1 = ISOPROPYLALCOHOL01  
Process NMR SPC File.


### <sup>1</sup>H NMR of Fish Oil

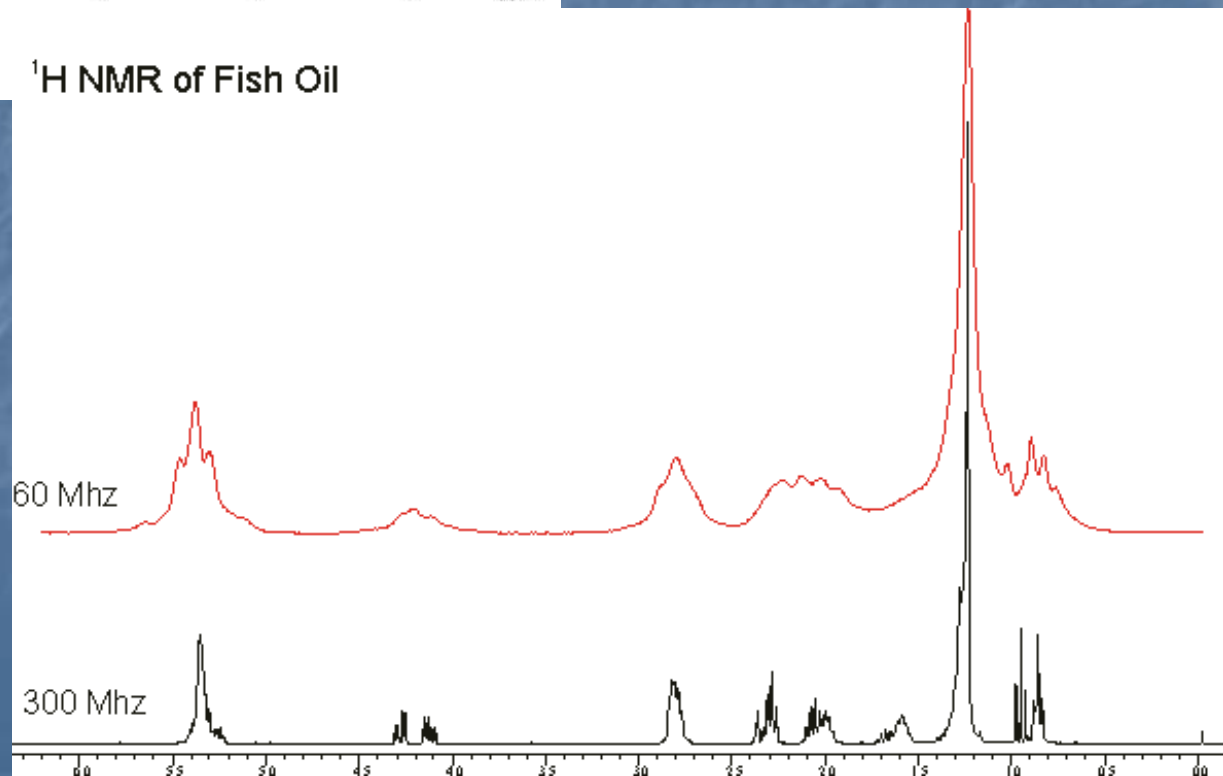



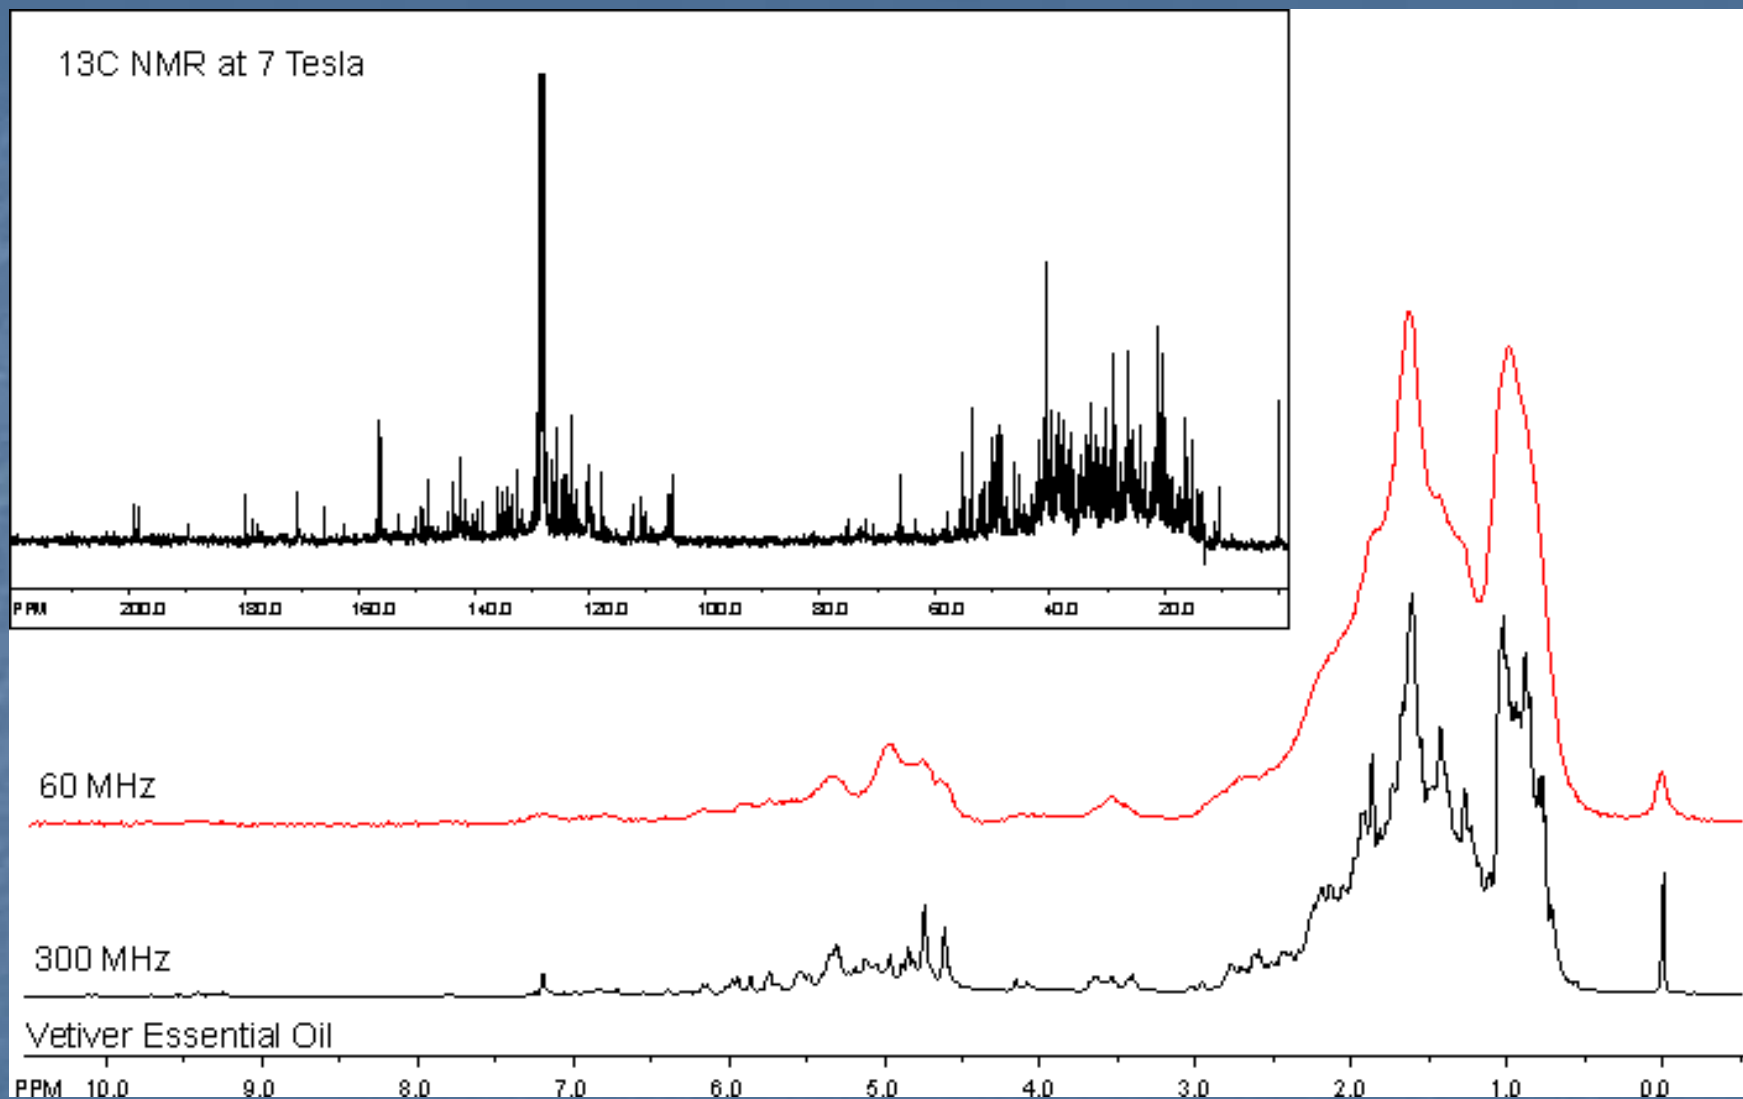

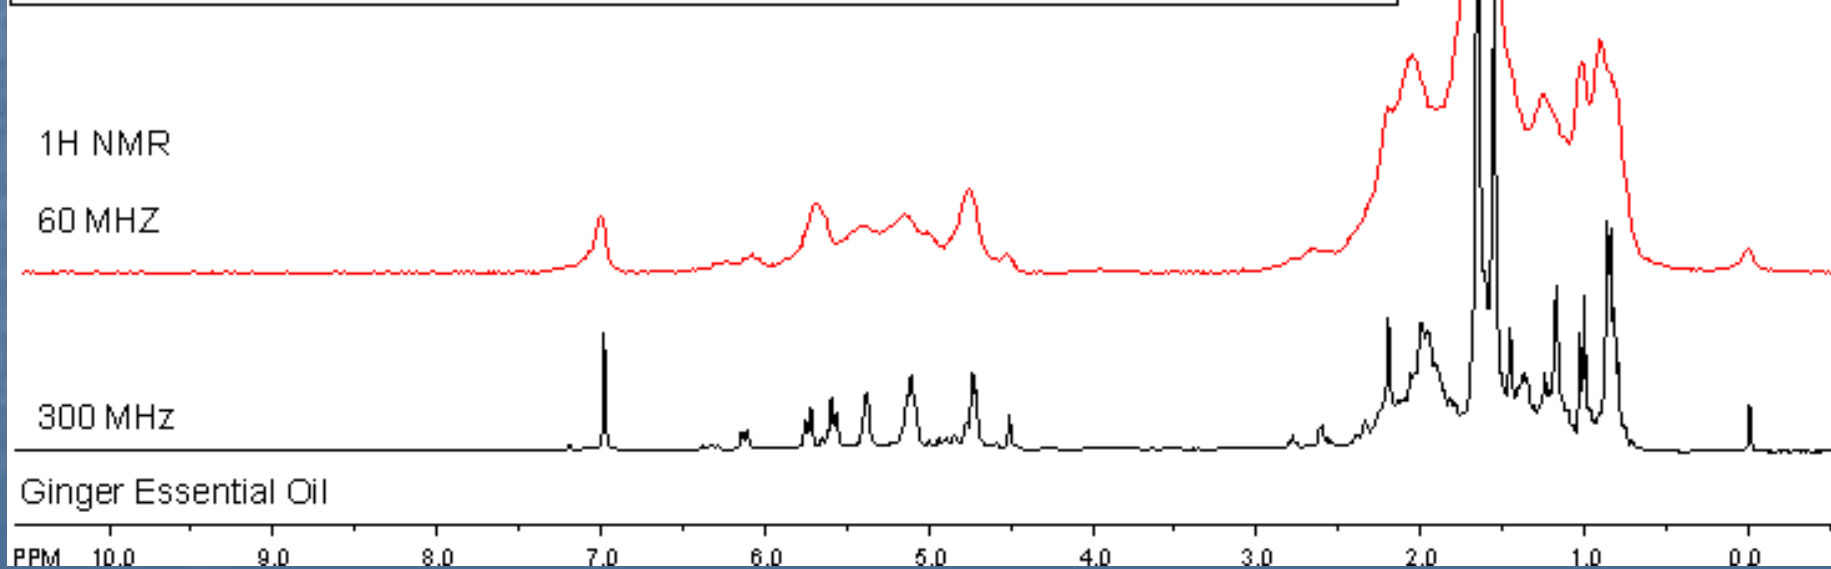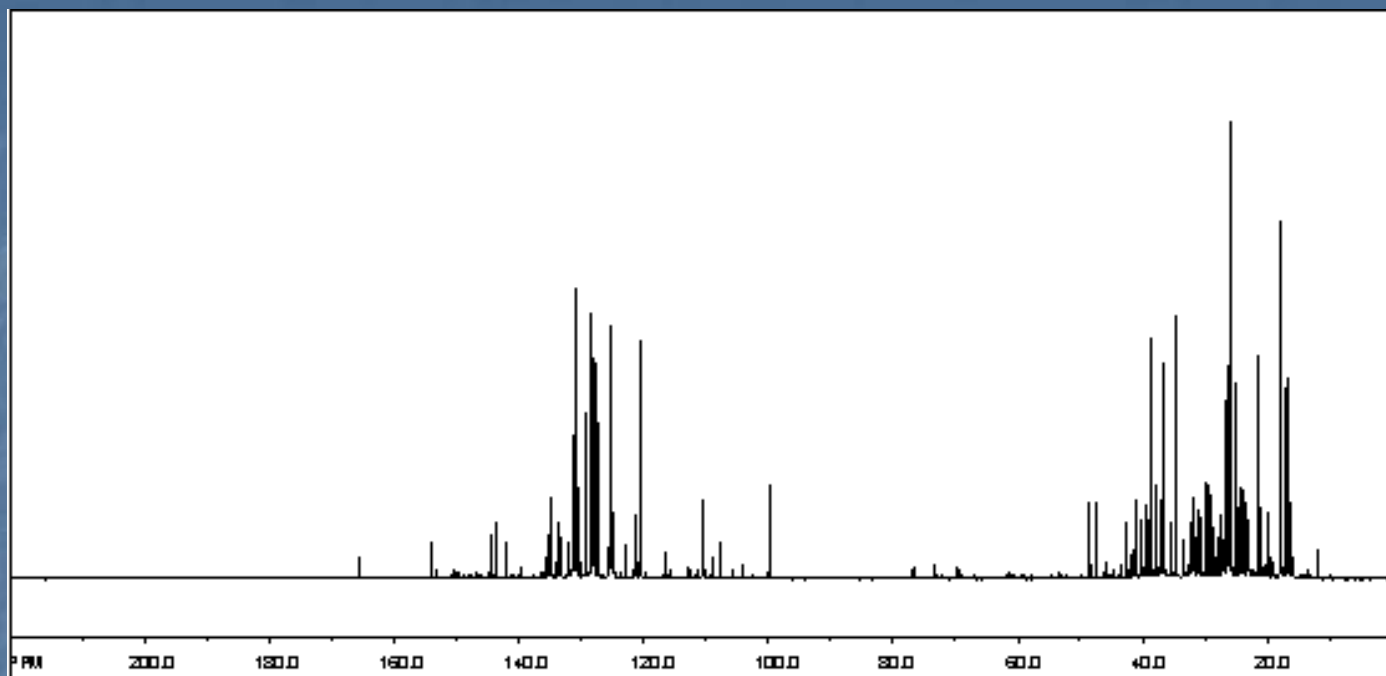

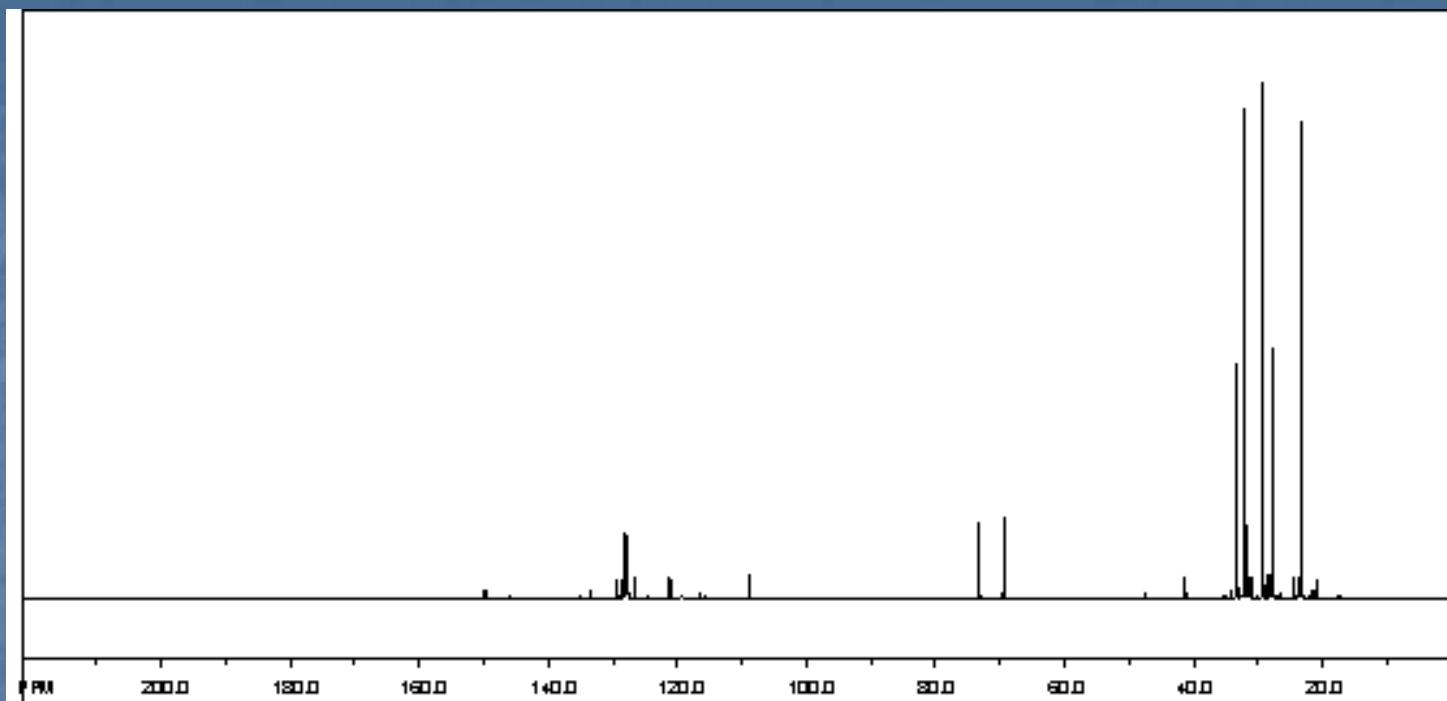

60 MHz


300 MHz

Eucalyptus Globulus Essential Oil

PPM 10.0 9.0 8.0 7.0 6.0 5.0 4.0 3.0 2.0 1.0 0.0



<sup>13</sup>C NMR at 7 Tesla

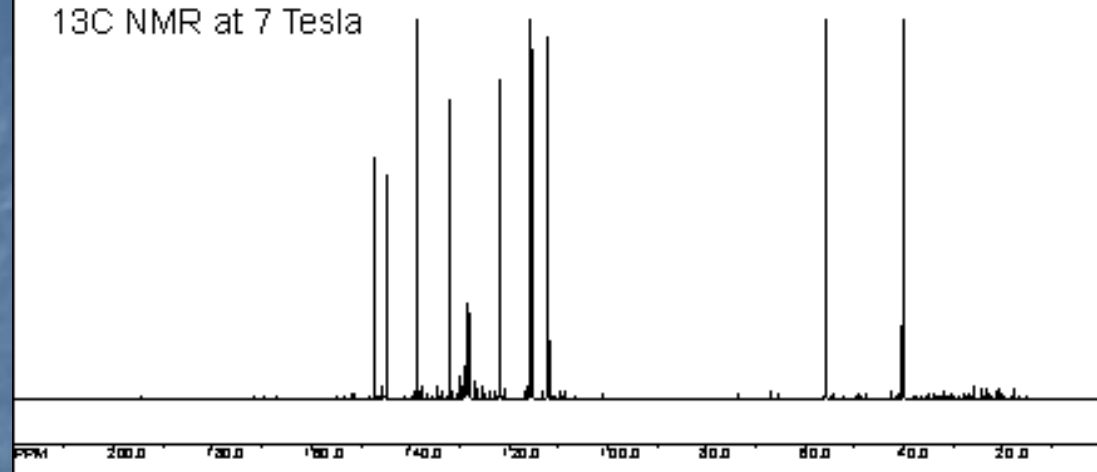



<sup>1</sup>H NMR

60 MHz


300 MHz

Cinnamon Leaf Essential Oil

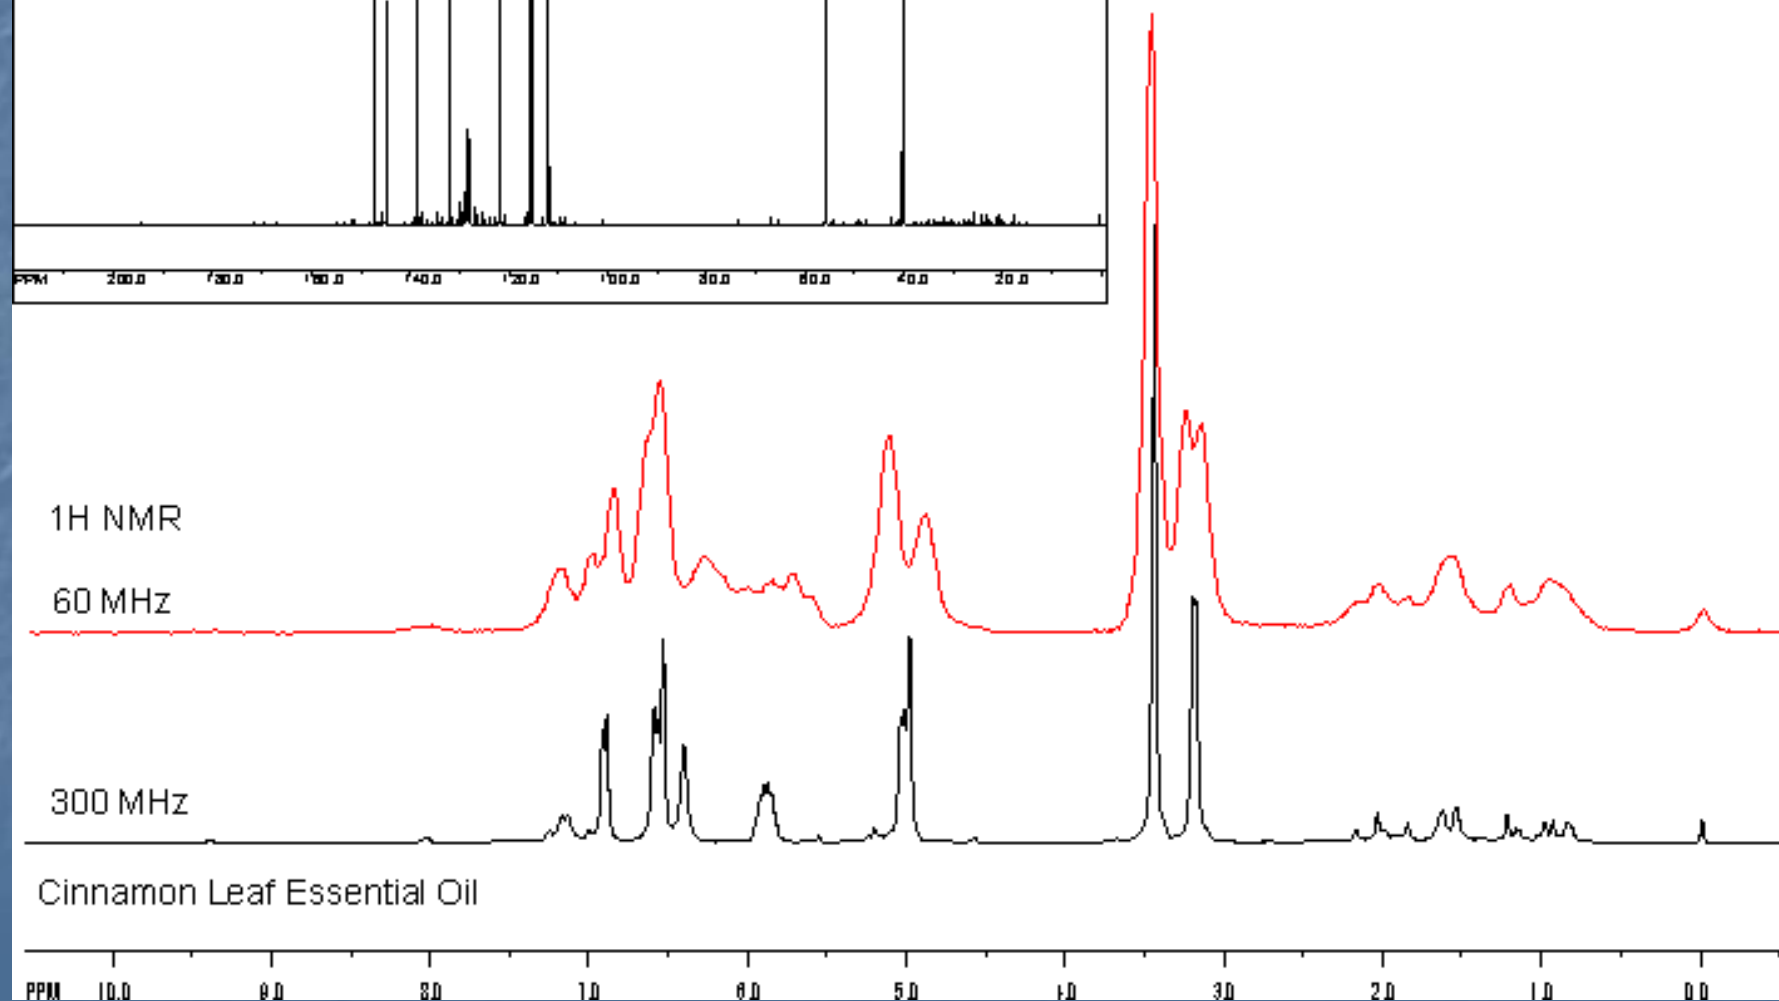





Diesel Fuels

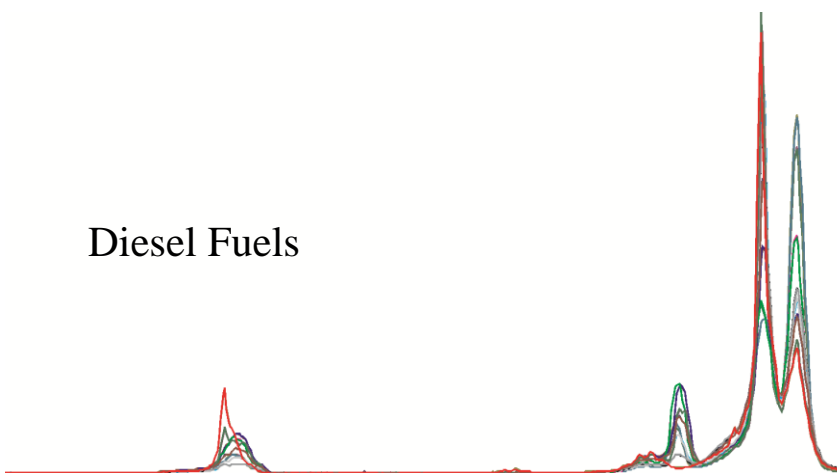


Biodiesels

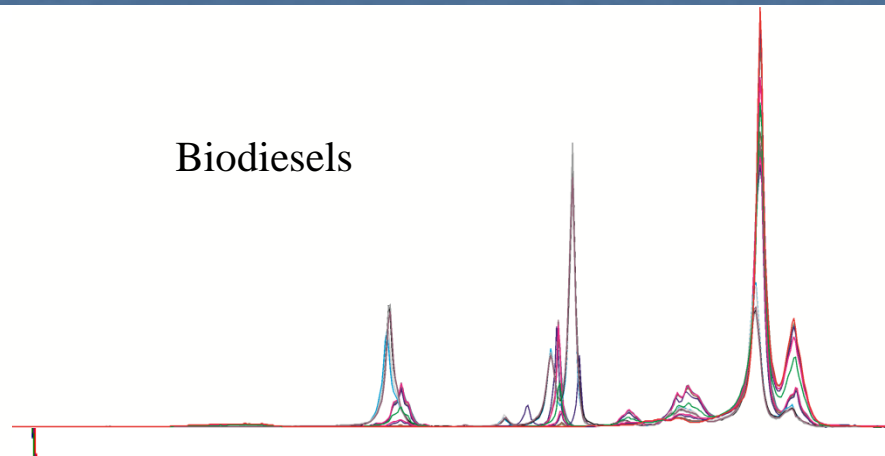


Ethyl-benzene  
Diethyl-benzene

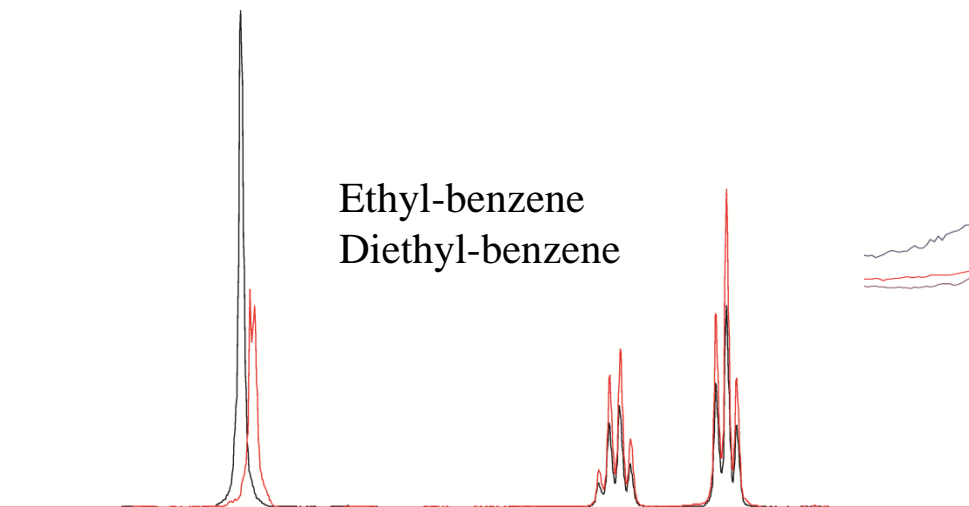


Vinegar and Alcohol Fermentation

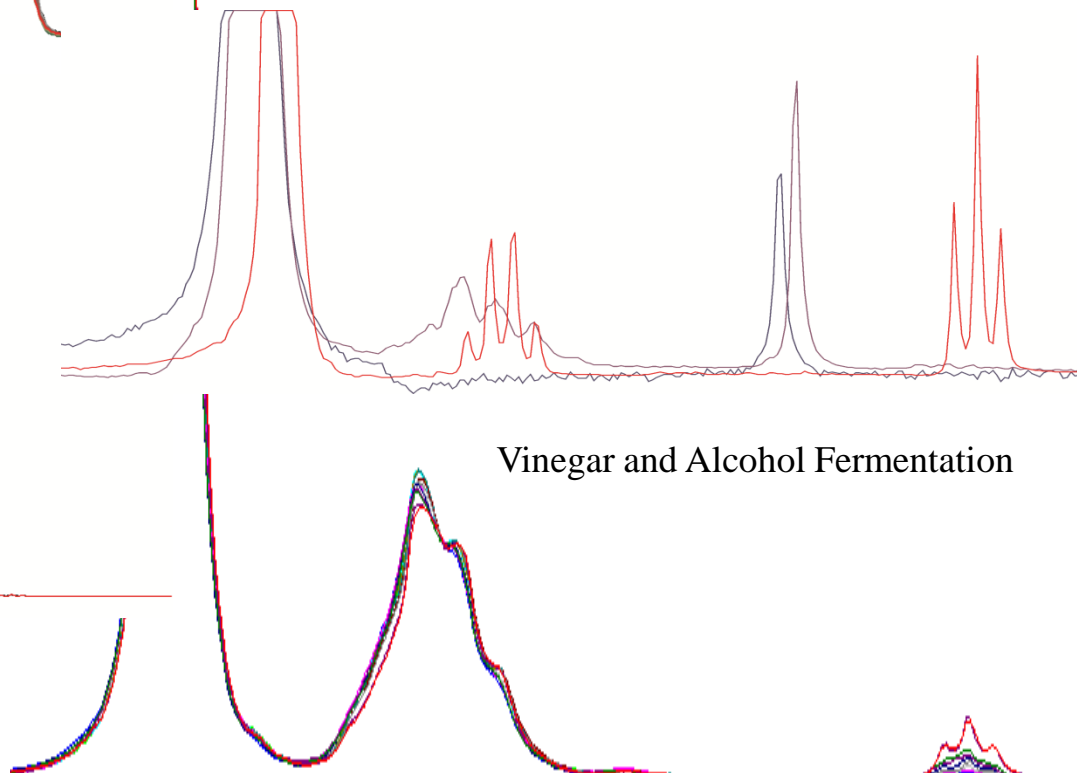





## Gasoline $^1\text{H}$ NMR

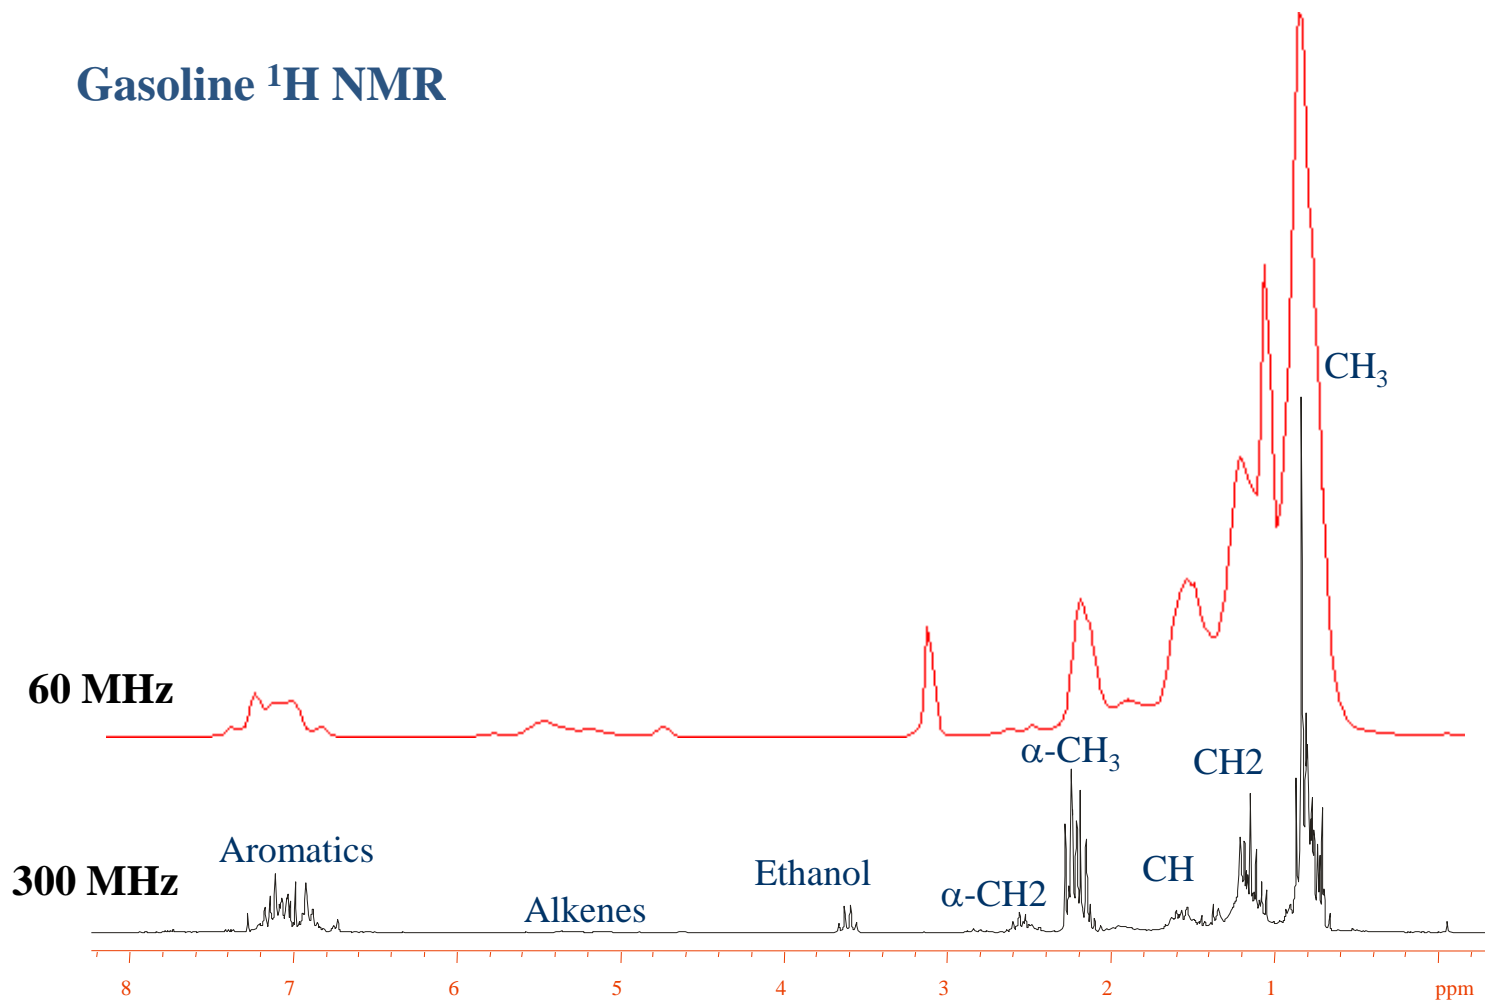






## Typical Variability Observed in Gasoline Blending

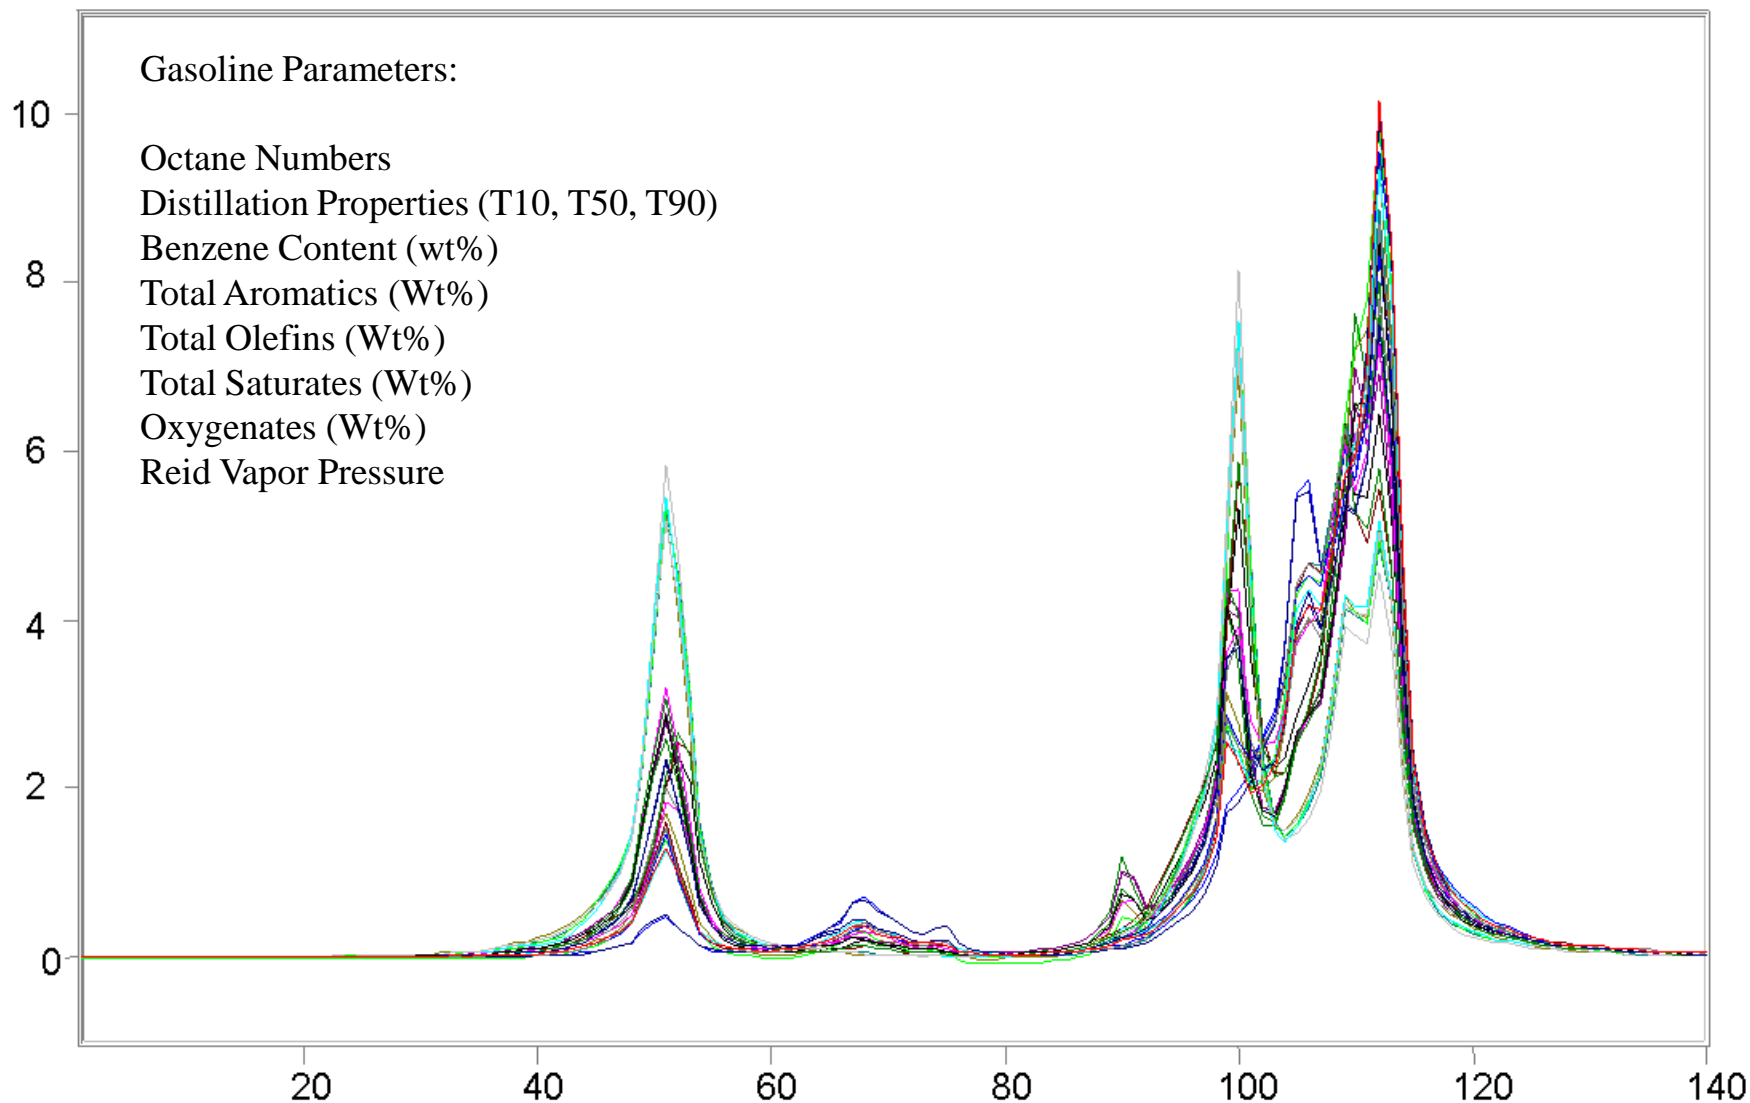



## Advantages and Disadvantages of NMR Applied to Process Control

### Advantages:

Non-Optical Spectroscopy

No Spectral Temperature Dependence

Minimal Sampling Requirements

Spectral Response to Sample Chemistry is Linear

Chemical Regions of NMR Spectra are Orthogonal

Entire Volume is Sampled by the RF Experiment

Water is in Distinct Region and can be digitally removed

Detailed Hydrocarbon information is readily observed.

Fundamental Chemical Information Can be Derived Directly from Spectrum.

Colored/Black Samples Readily Observed Without Impact

### Disadvantages:

Solids Cannot be Observed in a Liquid Stream


Individual Molecular Component Sensitivity Not Observed Directly in the Spectrum.

Low Sensitivity to Impurities – Quantitative > 500 ppm.

Sensitive to Ferromagnetics.

Sample Viscosity Causes Decrease in Resolution

Non-Hydrogen Containing Species are Not Observed (Exceptions Na, P, F, Al)



## PROCESS NMR ASSOCIATES


### Application: Closed Loop Reformer Control - Installed 1998

Reformer Capacity: 34,000 Barrels per Day

Control Strategy: Control on MON and Benzene Content



NMR Analysis: 2 Minute Analysis

NMR PLS Outputs: RON, MON, Benzene (Wt%) Total Aromatics (Wt%)

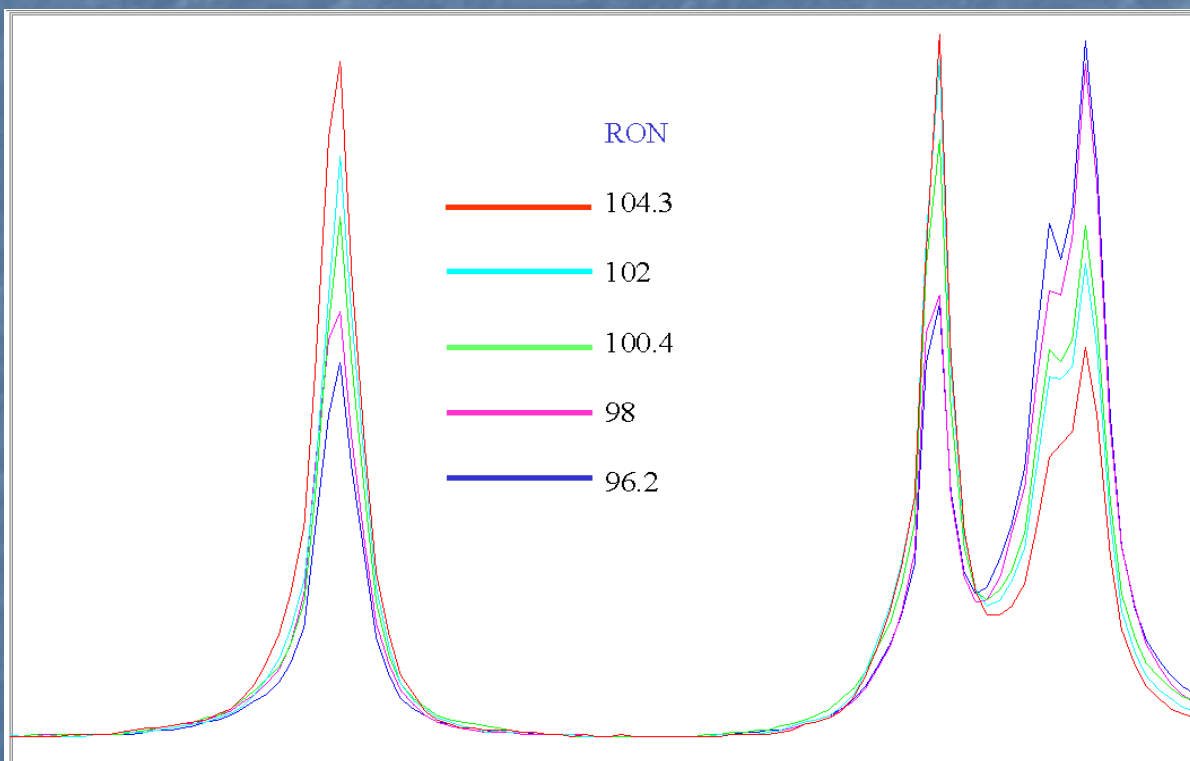


Variation of Reformate Processed  $^1\text{H}$  NMR Data Observed with Changing Research Octane Number

Current Model on System

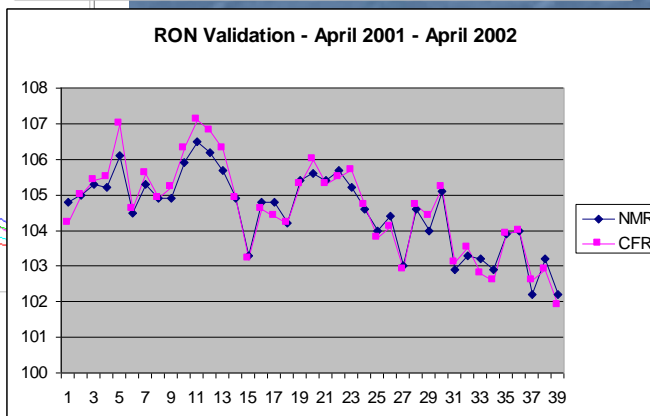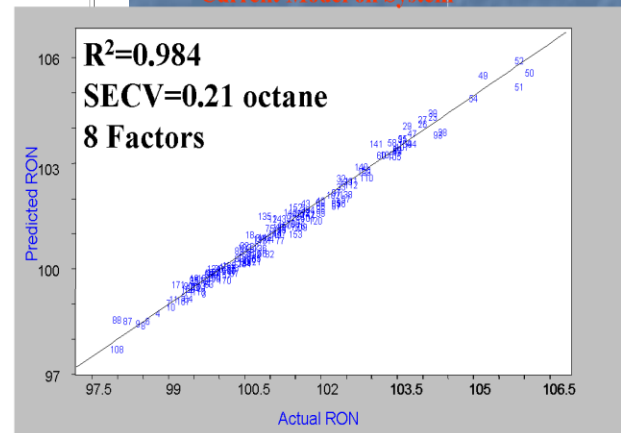





## PROCESS NMR ASSOCIATES

### Application: Steam Cracking Optimization Installed 2000


Cracker Facility Capacity: 600,000 Tonnes per Year

Control Strategy: Feed Forward Detailed Hydrocarbon Analysis to SPYRO Optimization


NMR Analysis: 3-4 Minute Cycle (Single Stream)


NMR PLS Outputs: Naptha – Detailed PIONA

C4-C10 normal-paraffin, iso-paraffin, aromatics, naphthenes

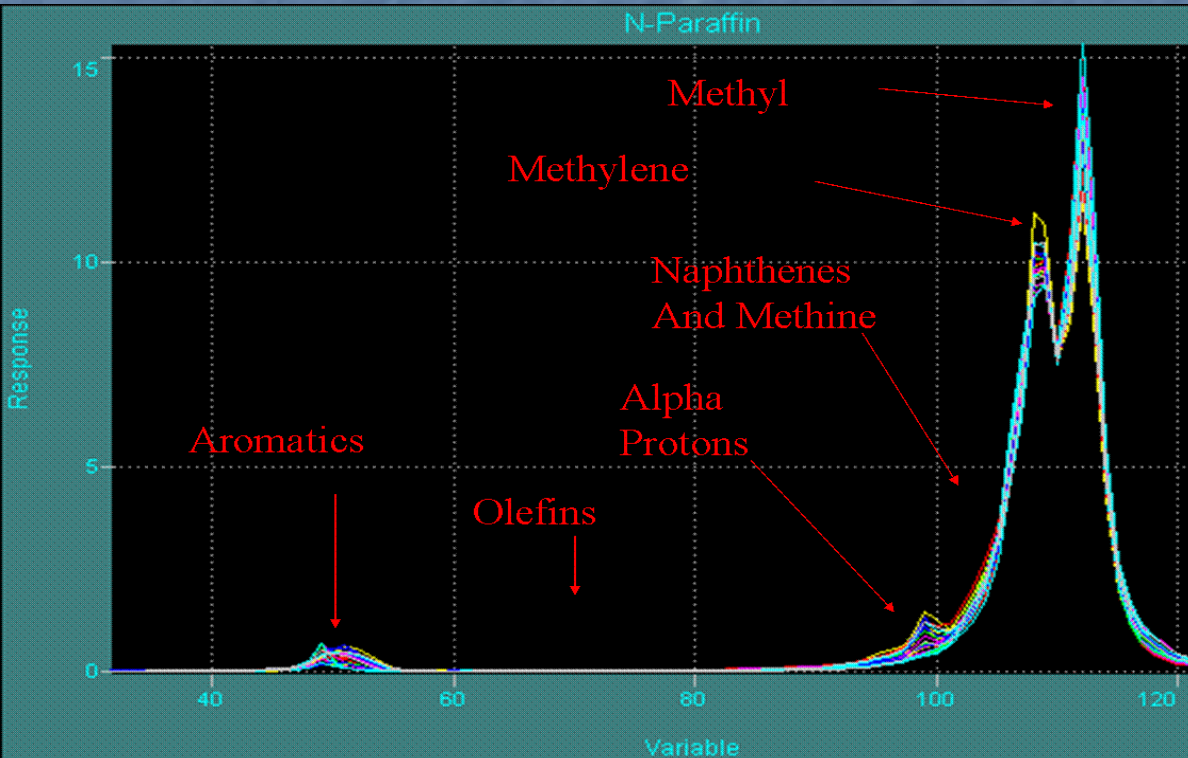


Spectral Variability Observed in Naptha Samples

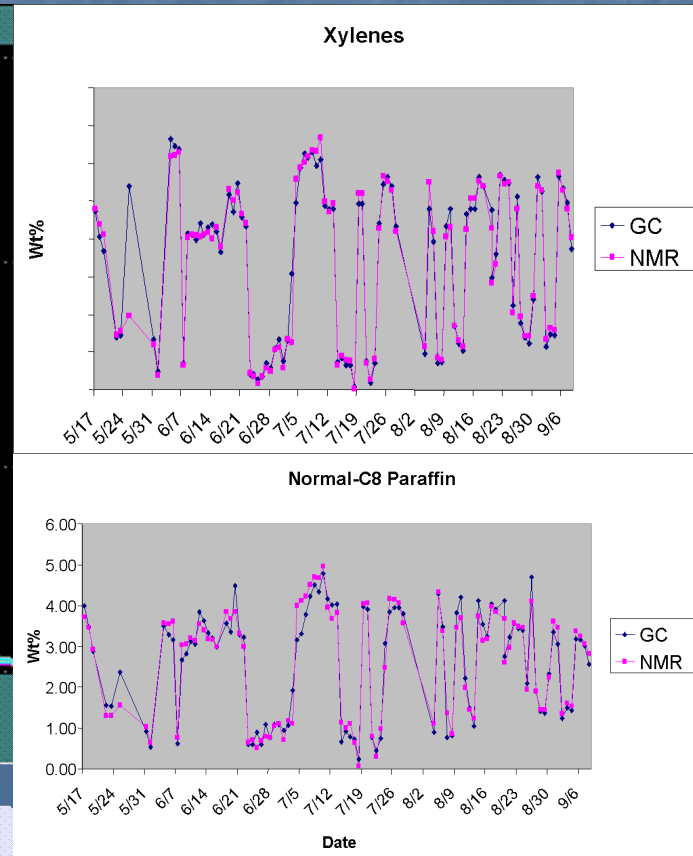





# PROCESS NMR ASSOCIATES

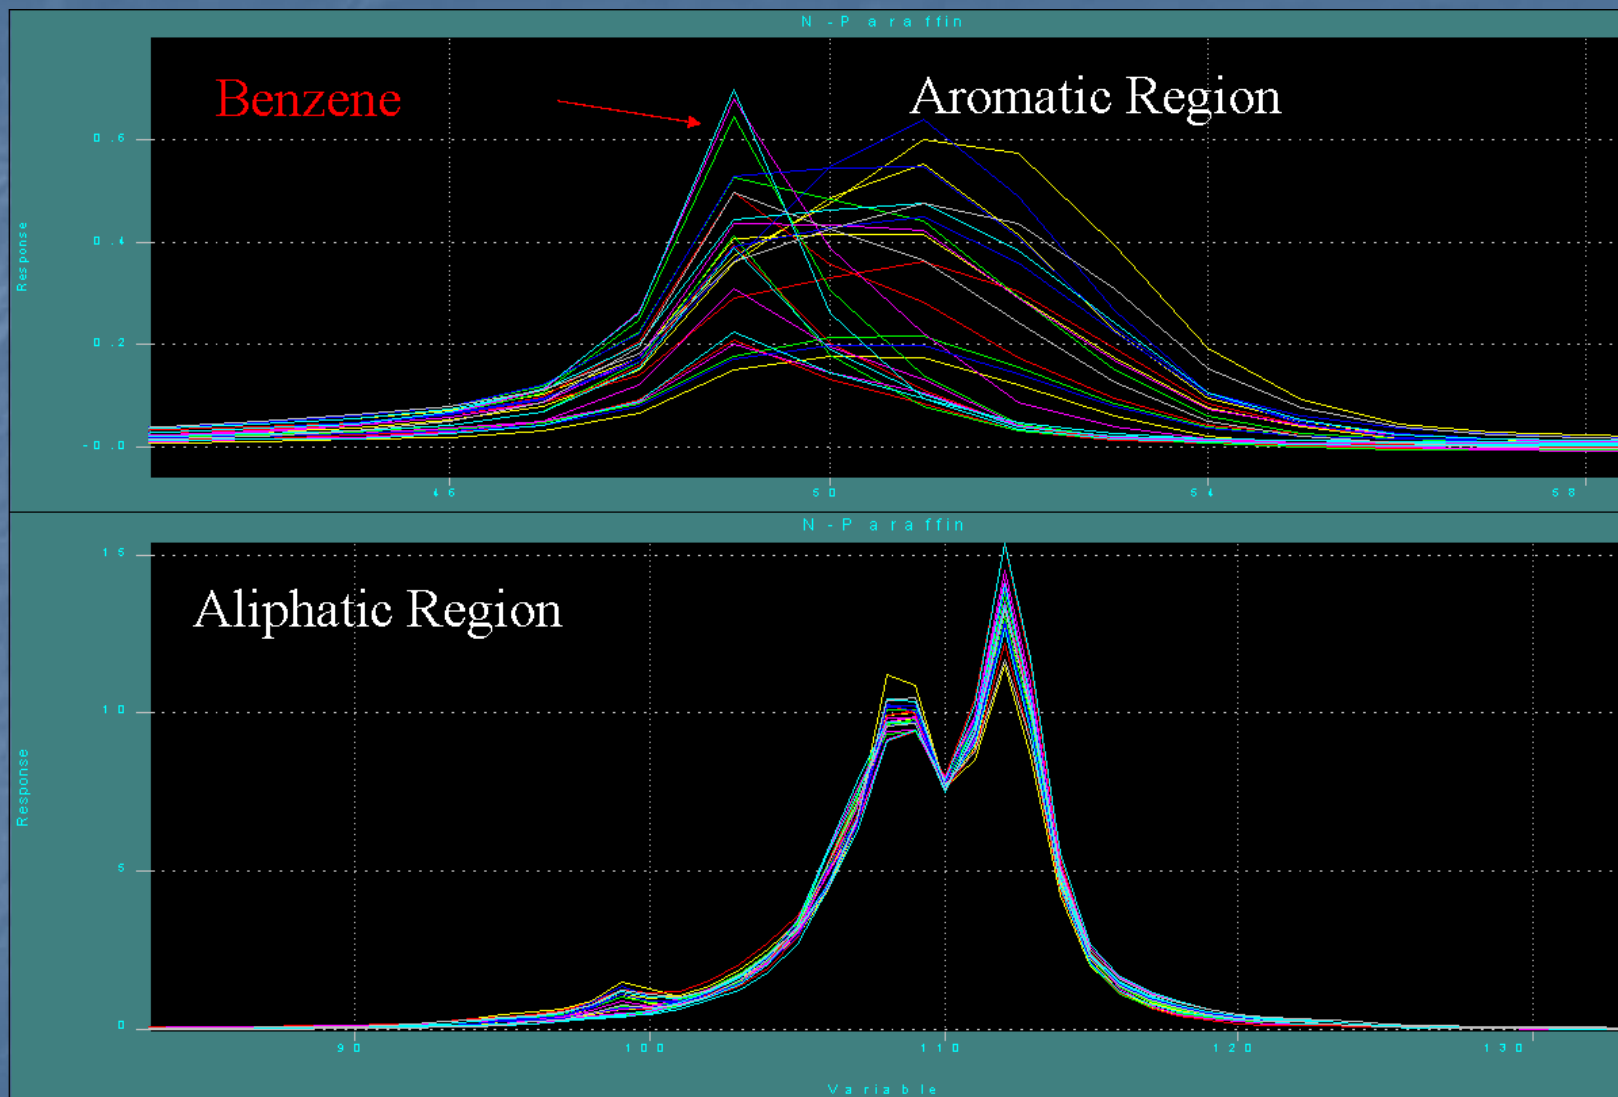


Spectral Variability in Aromatic and Aliphatic Regions




PROCESS NMR ASSOCIATES

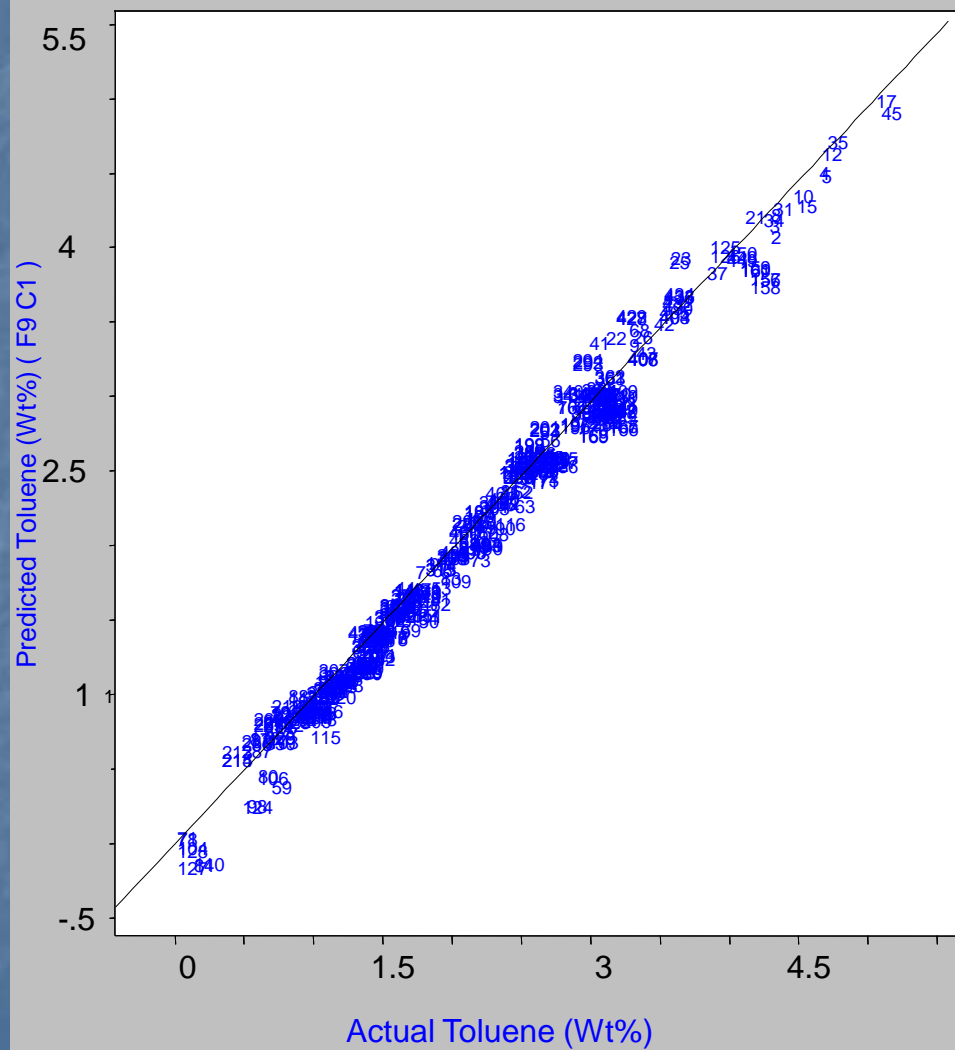


# Toluene

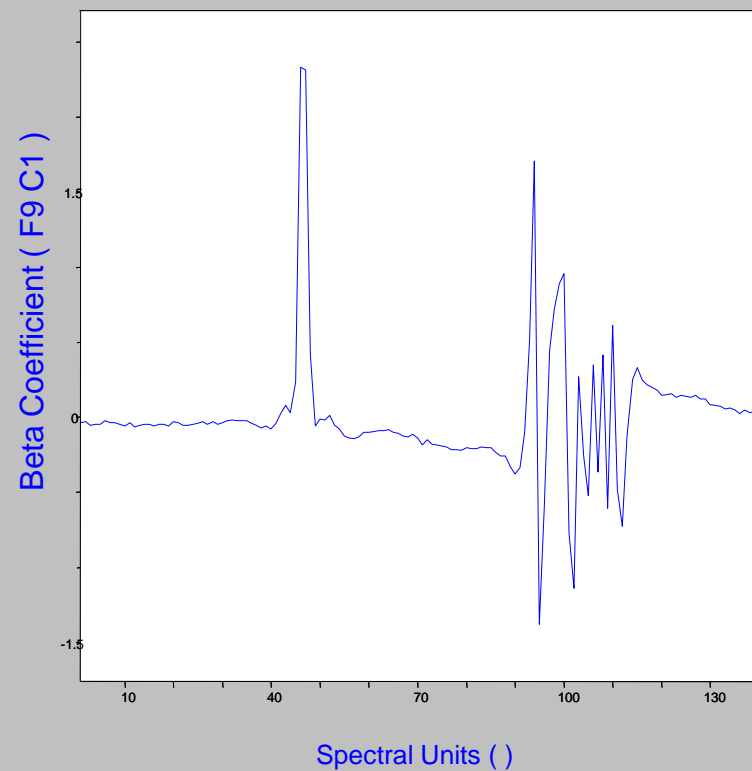





PROCESS NMR ASSOCIATES

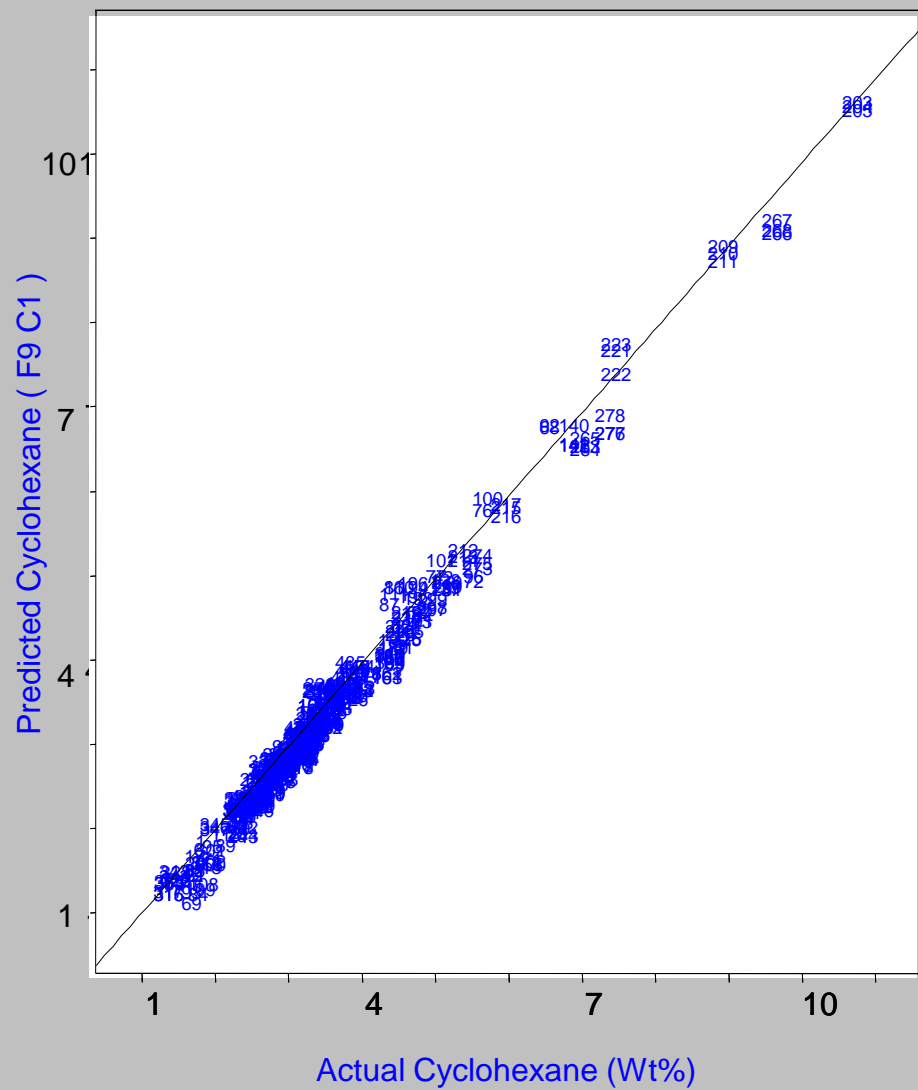


## Cyclohexane

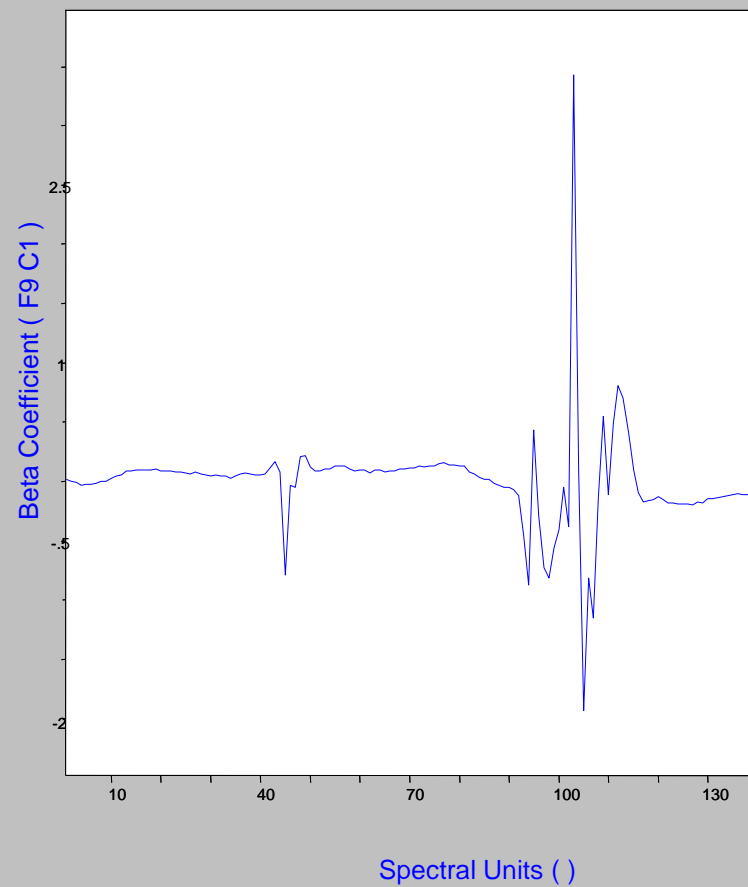





## Normal-C8 Paraffin

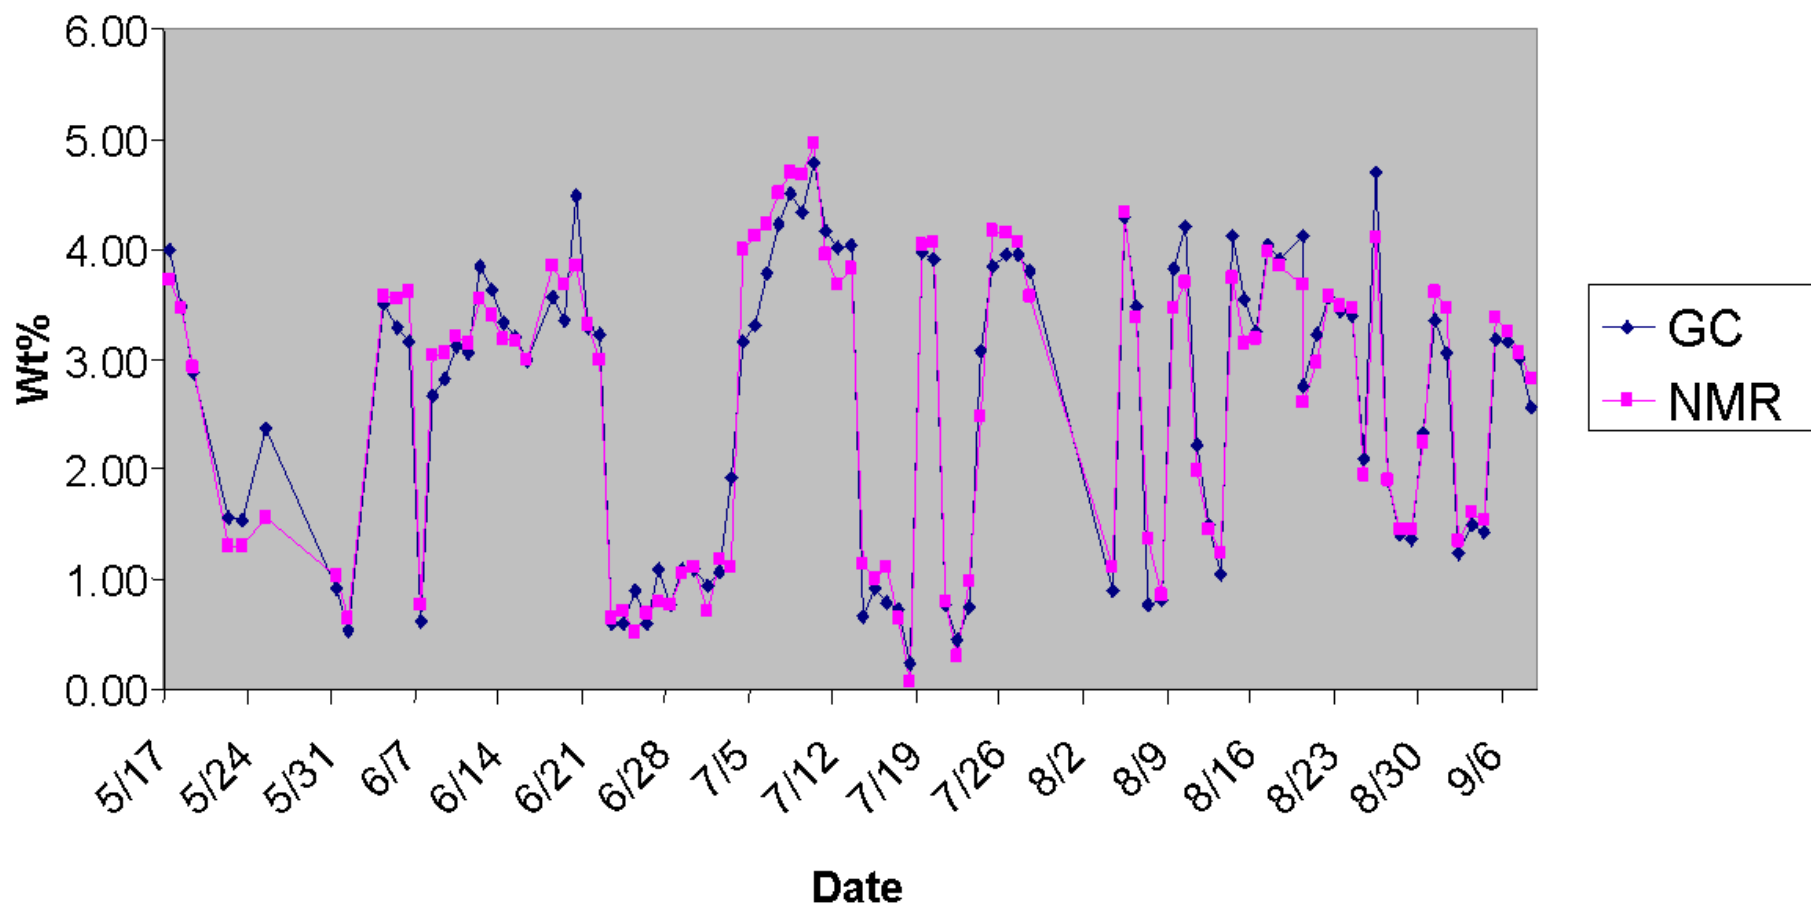








## Iso-C5 Paraffin

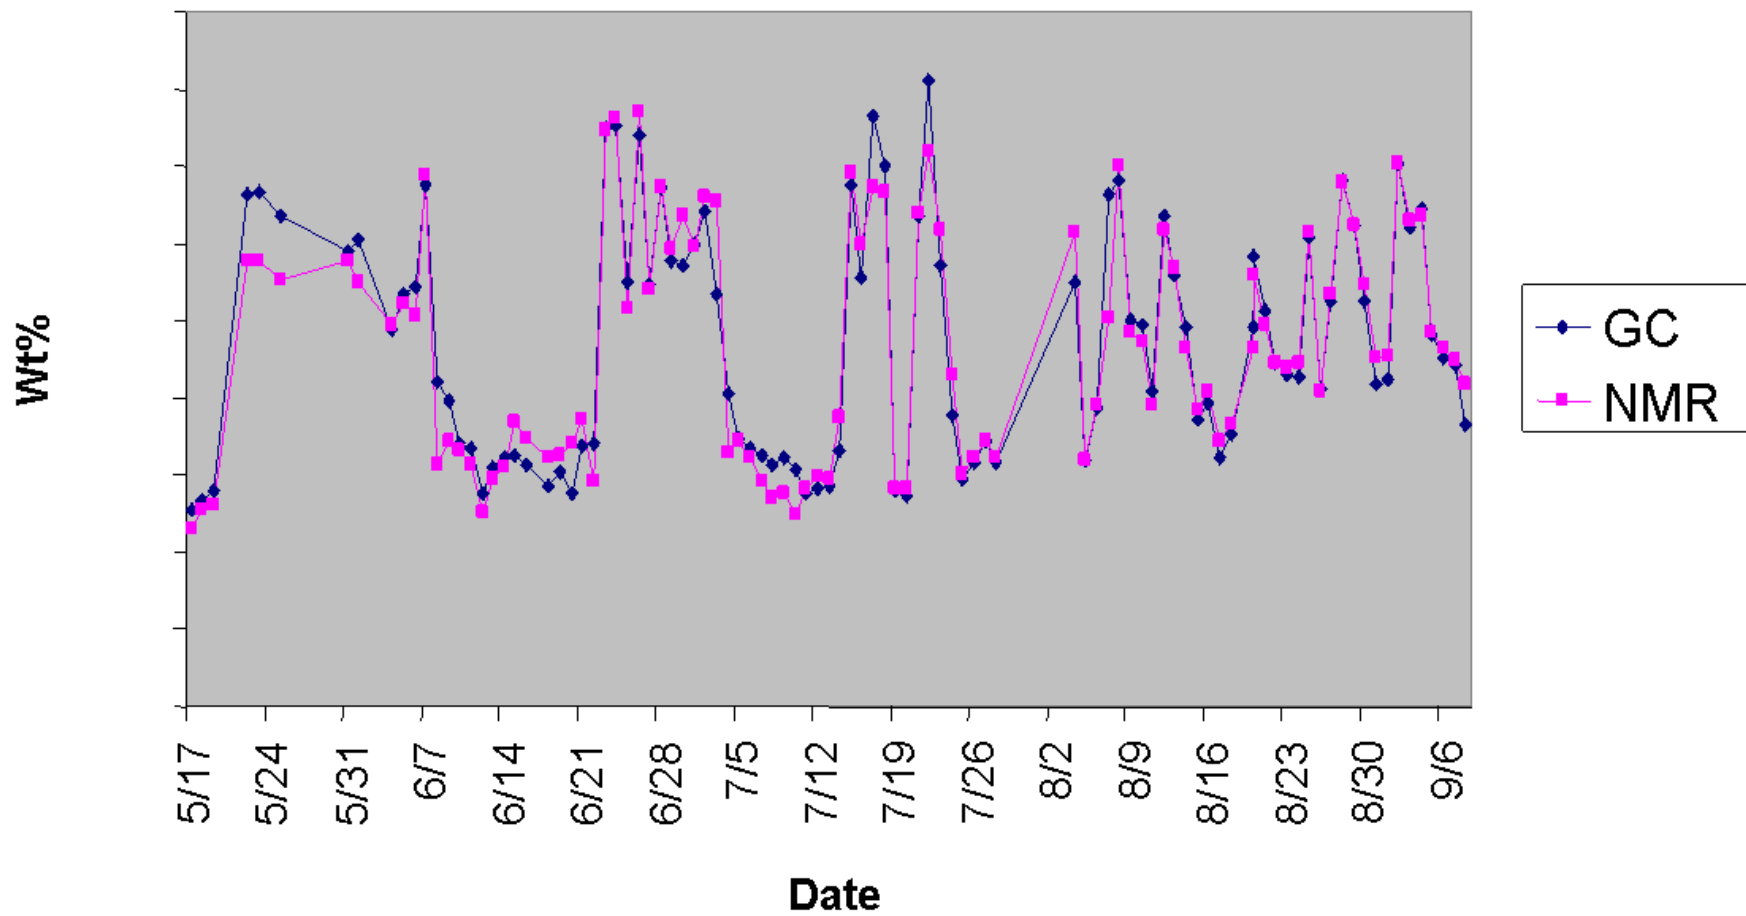





## Cyclopentane

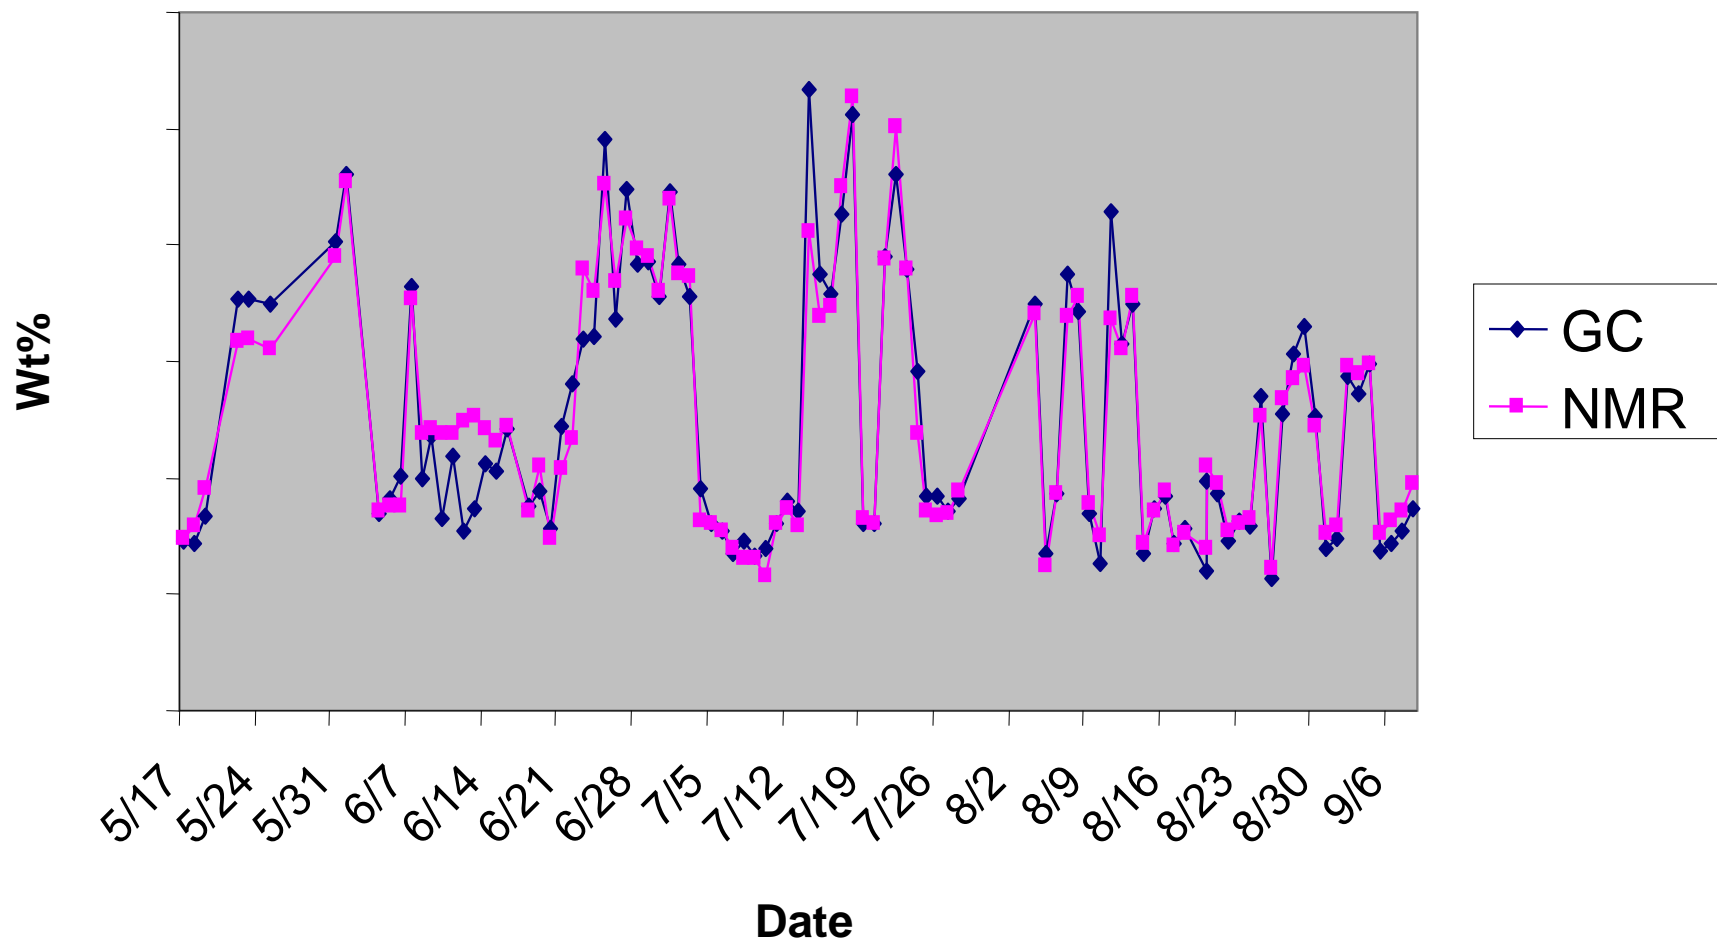




## Xylenes

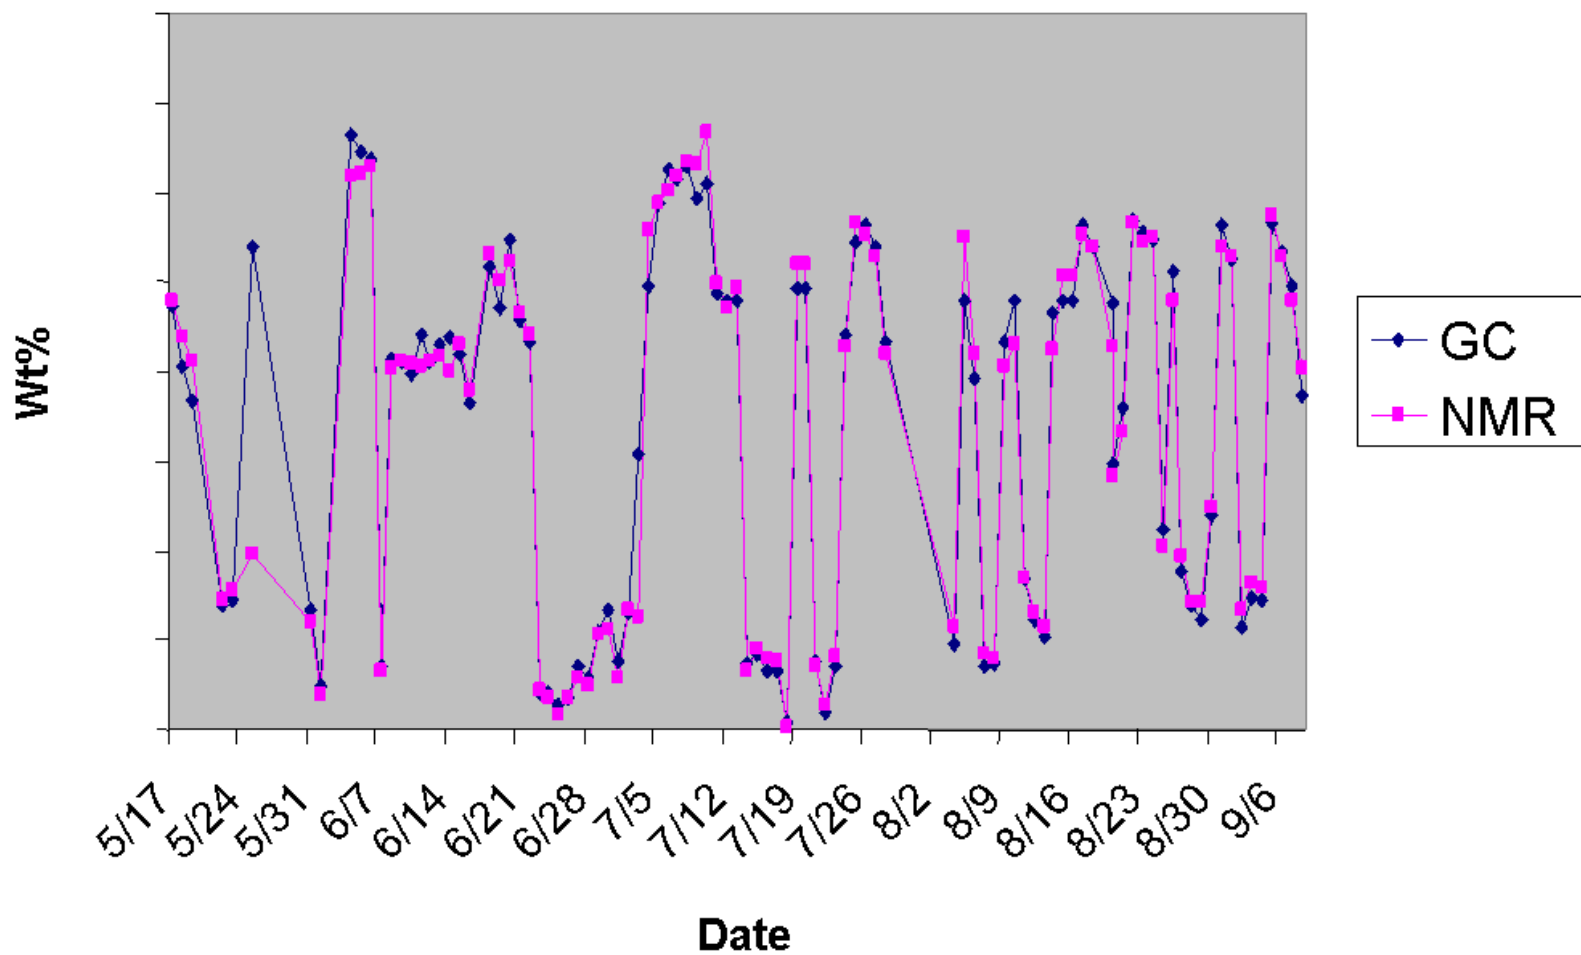





PROCESS NMR ASSOCIATES

## 96 Hours of NMR Process Output – iso-Paraffin Components

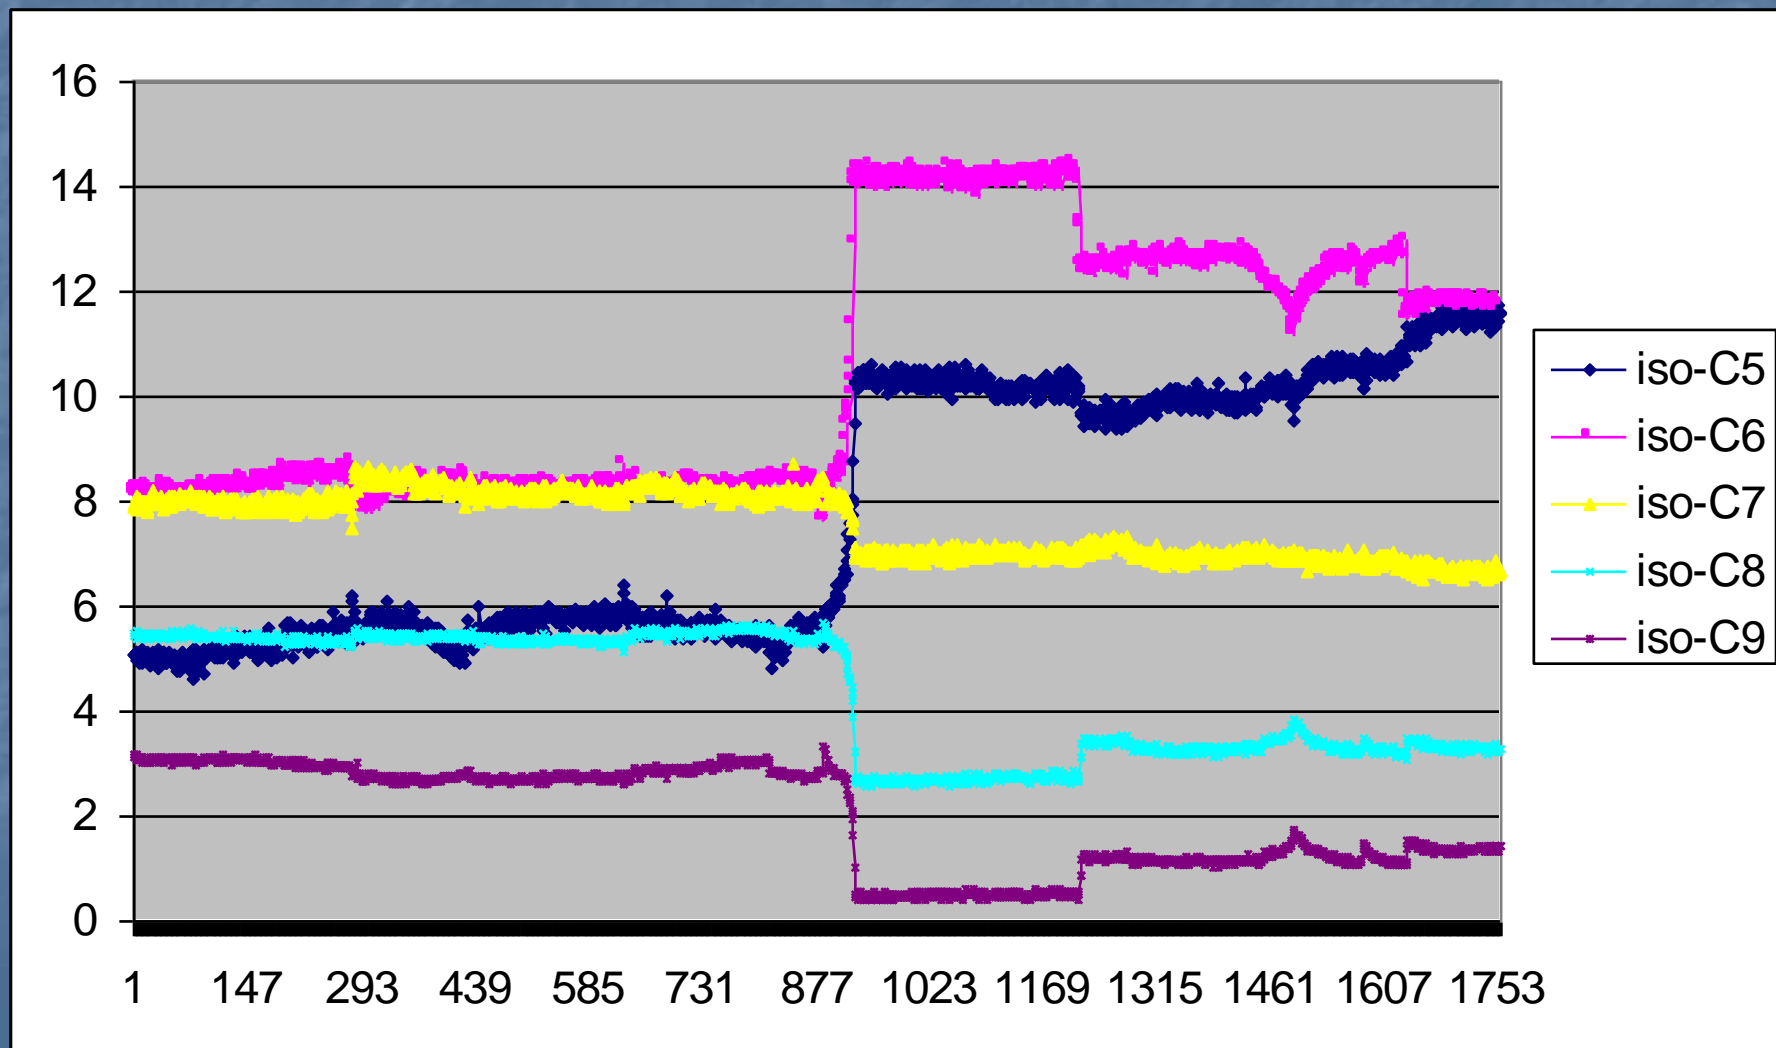




## 96 Hours of NMR Process Output – Aromatic Components


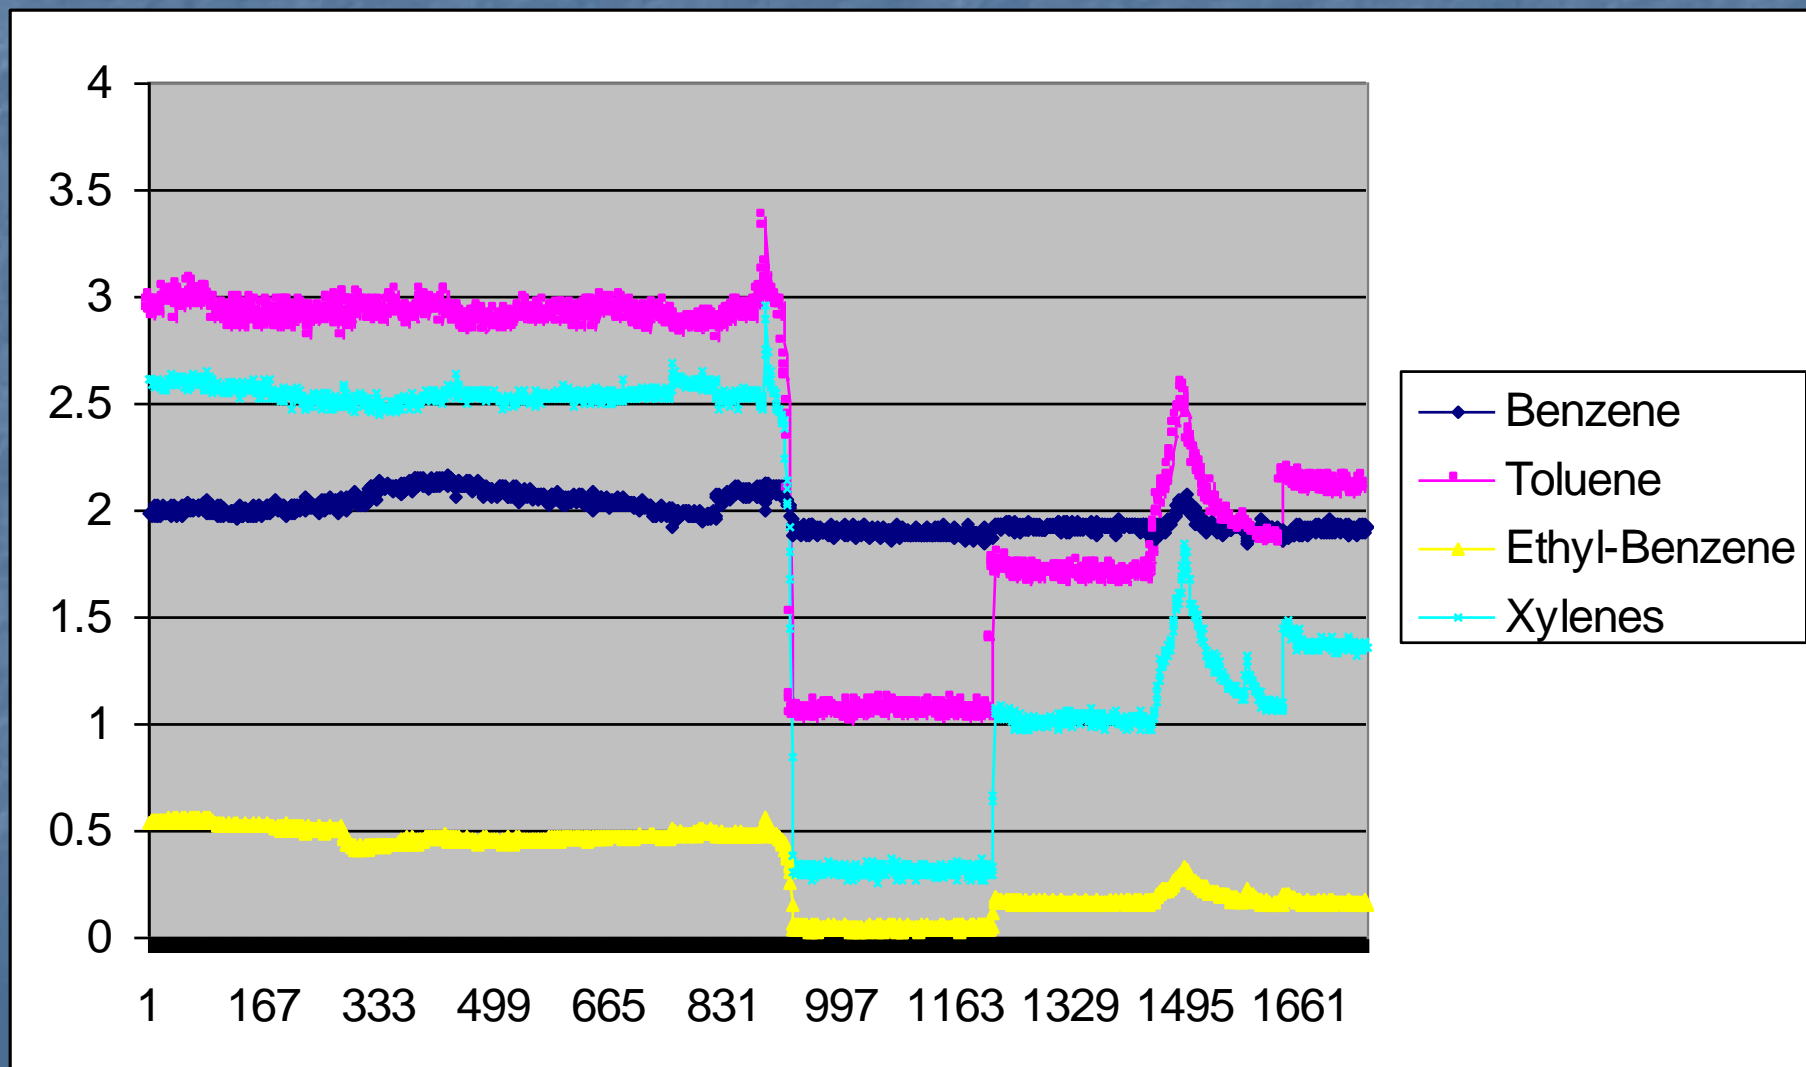









## Online NMR Applications Timeline


- 1993 - Development of Laboratory Based process NMR Methodologies
- 1995 - BTU Analysis of Refinery Fuel Gas
- 1995 - Sulfuric Acid Strength in Emulsion Zone of Stratco Acid Alkylation Unit
- 1999 - Diesel Blending System
- 1999 - Reformer Control System
- 2000 - Naphtha Cracker Feed Analyzer – Full GC PIONA
- 2000 - Crude Unit Analyzer
- 2000 - Crude Blending System
- 2001 - Gasoline Blending System,
- 2001 - Base Oil Manufacturing Analyzer
- 2002 - FCC Unit Analyzer

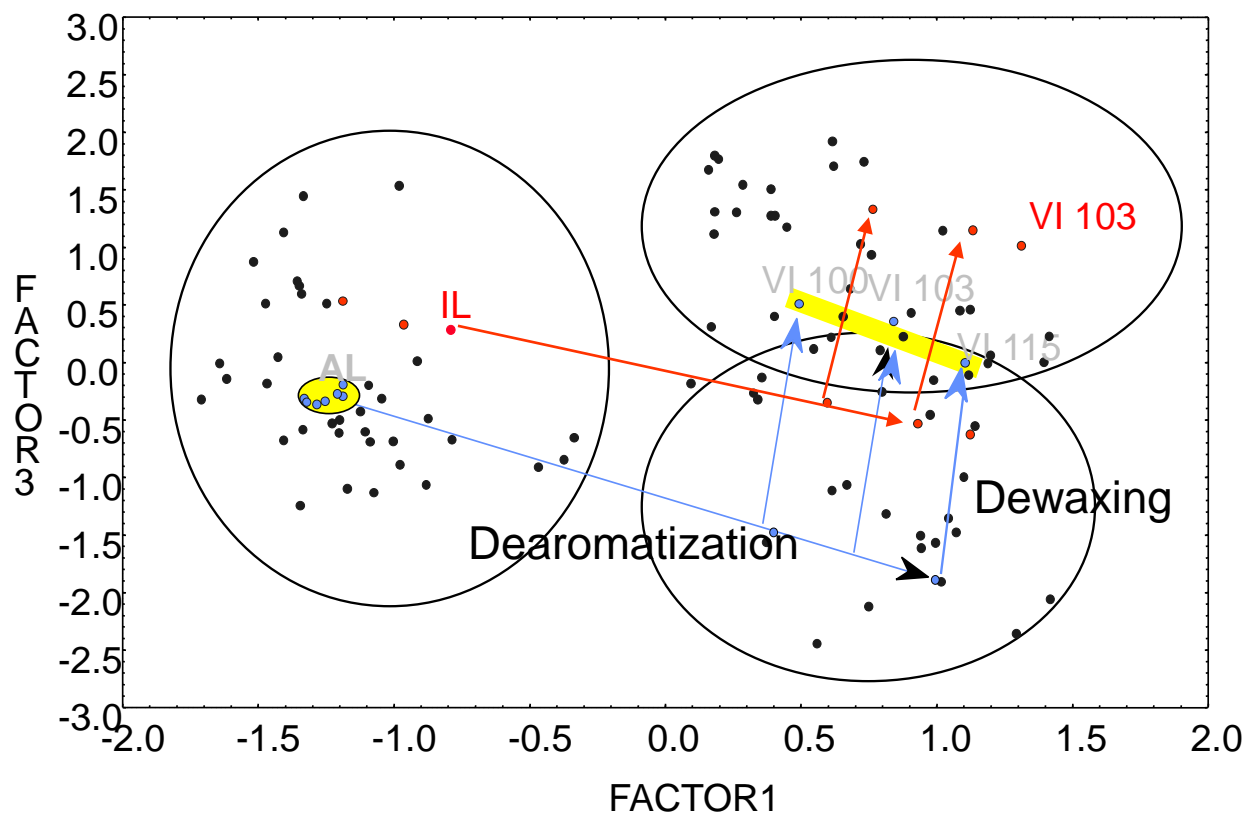


Base Oil Manufacturing – NMR Control


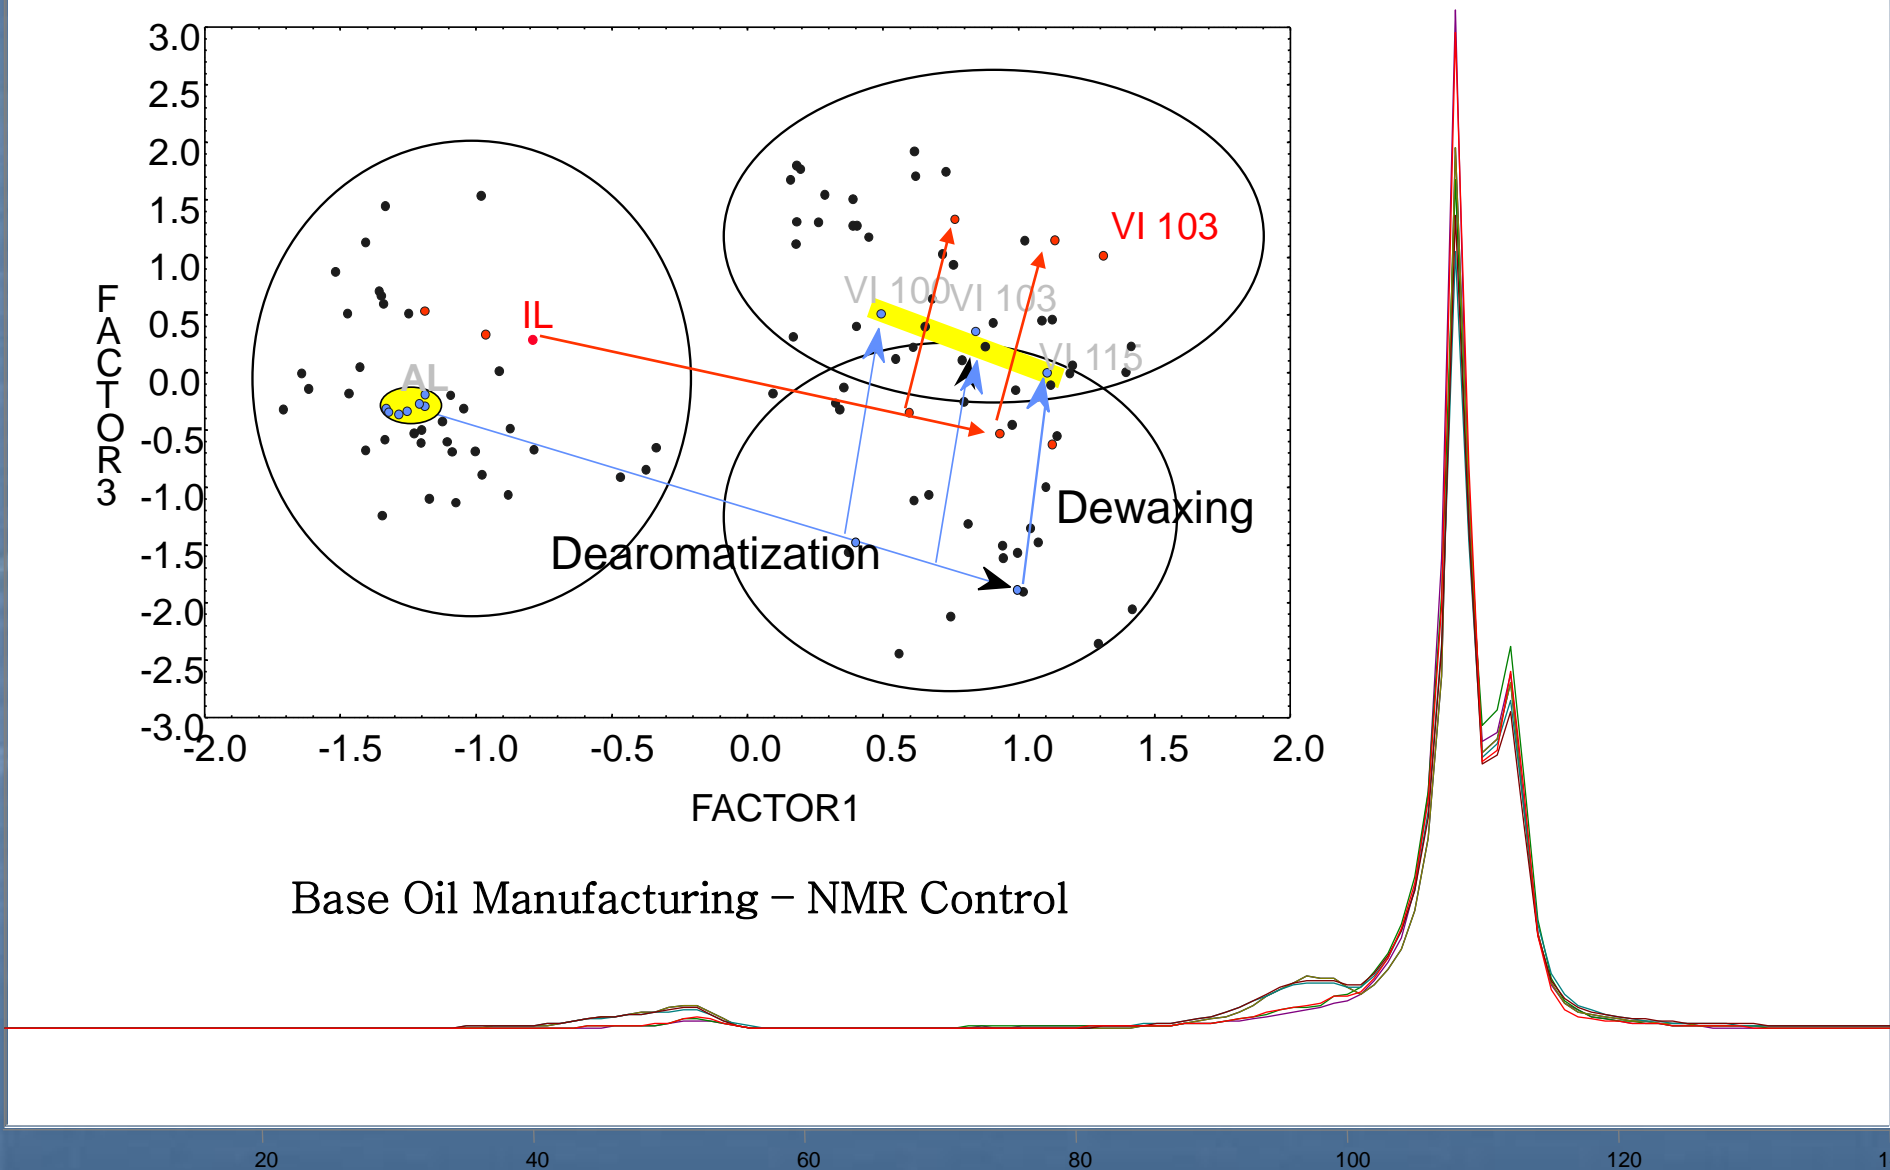


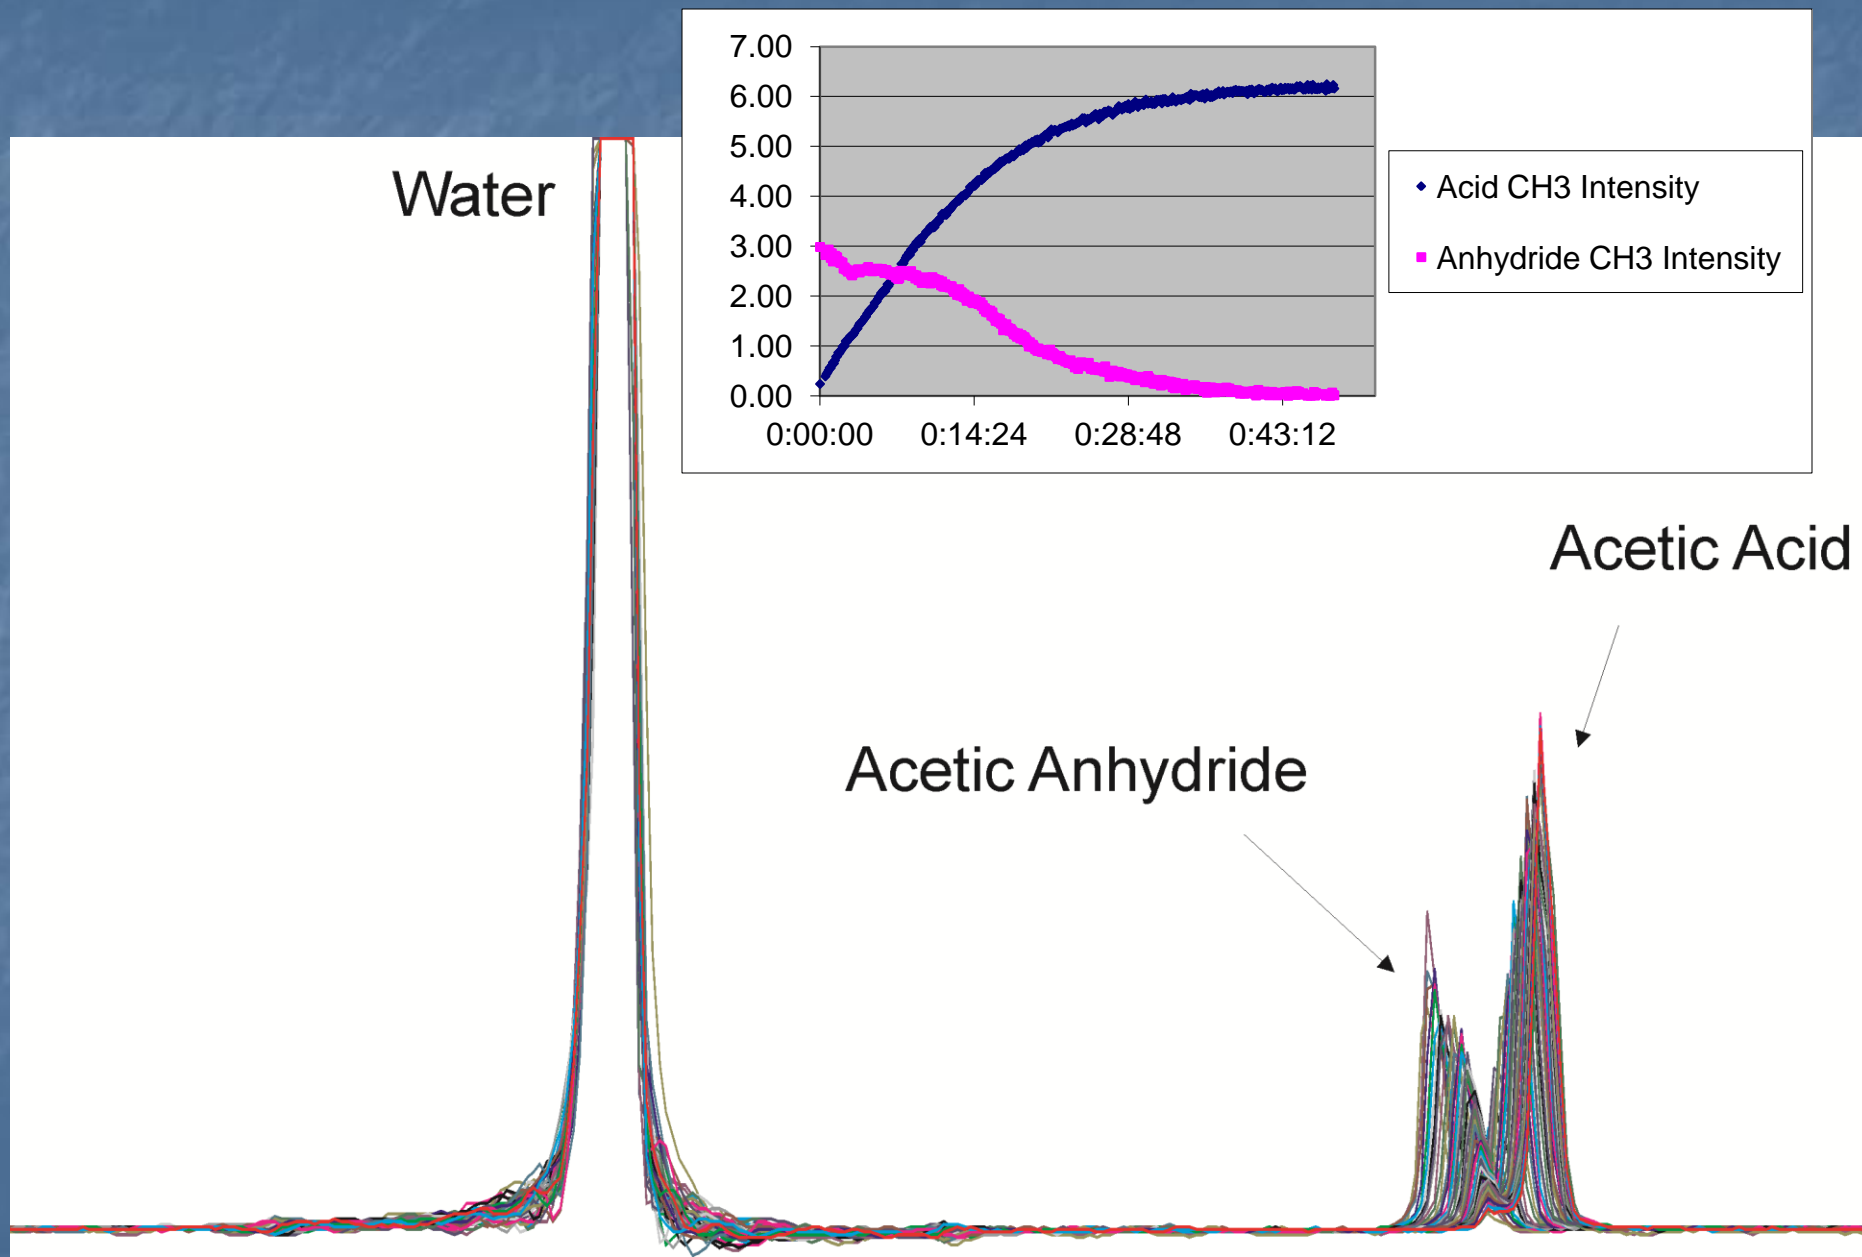




# PROCESS NMR ASSOCIATES

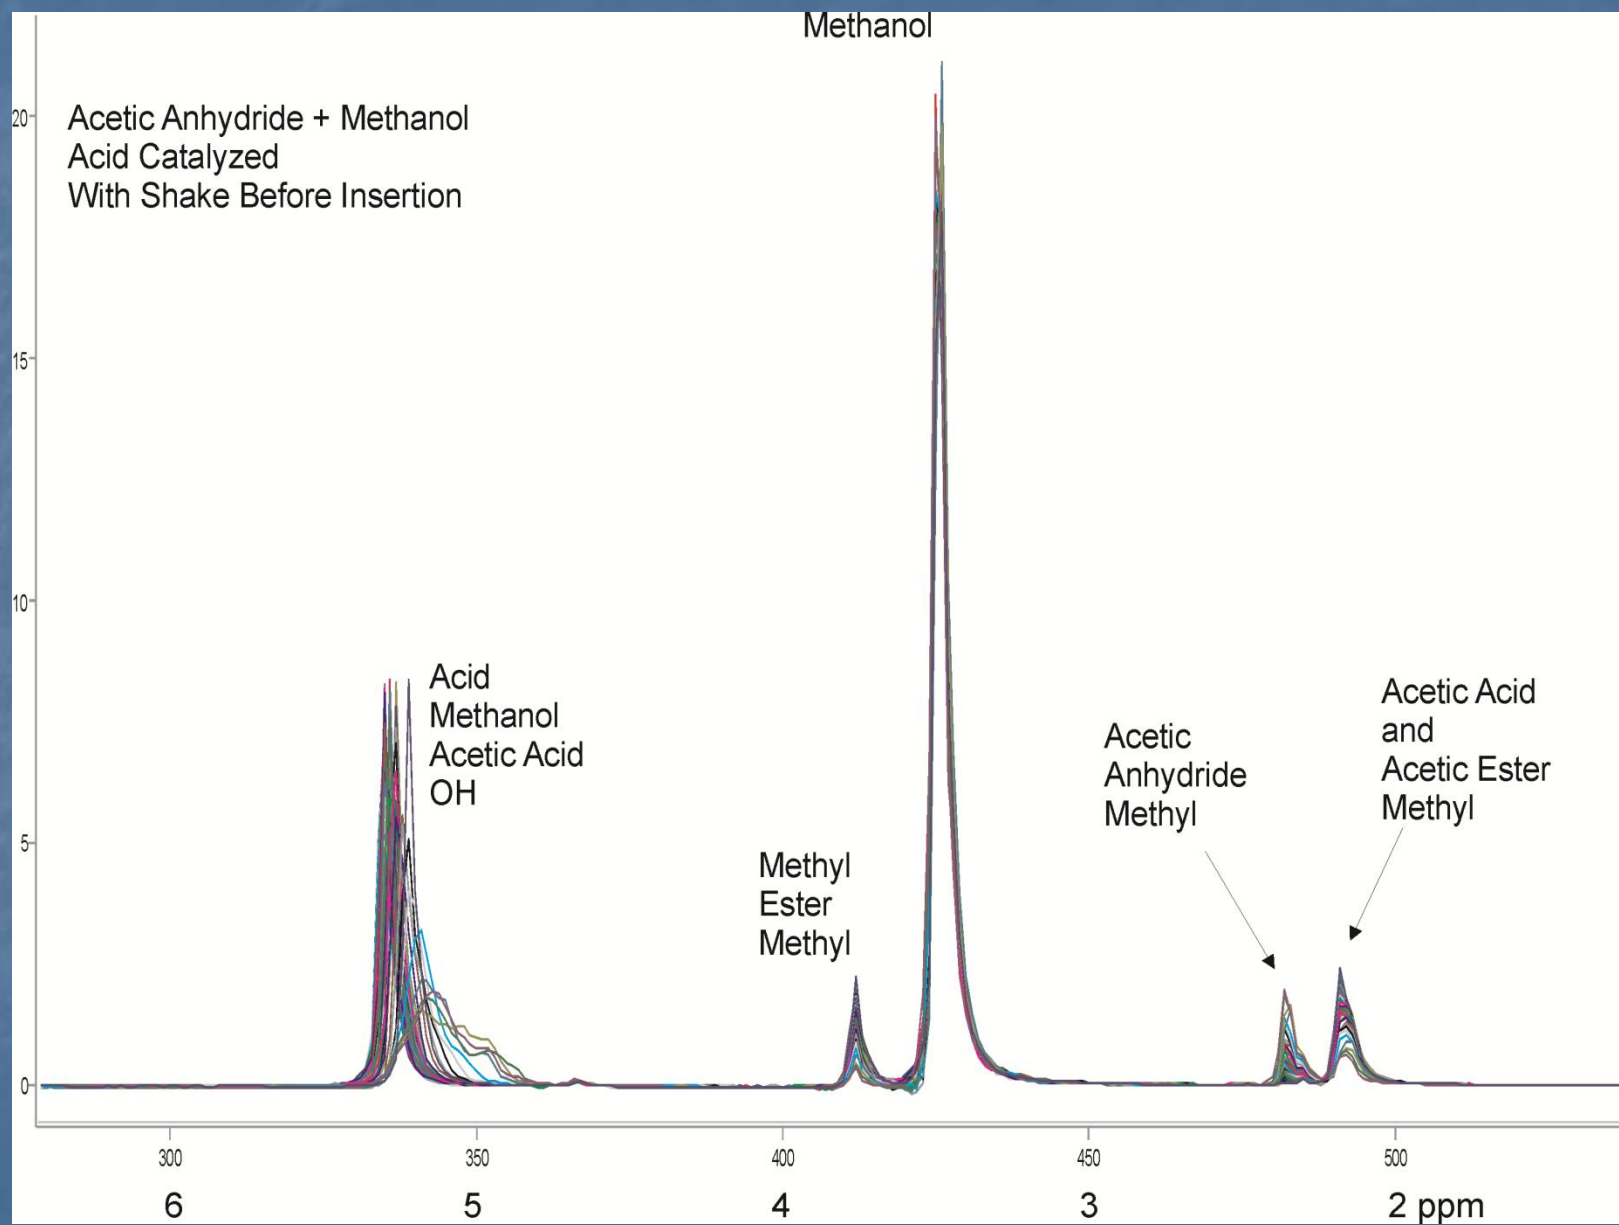


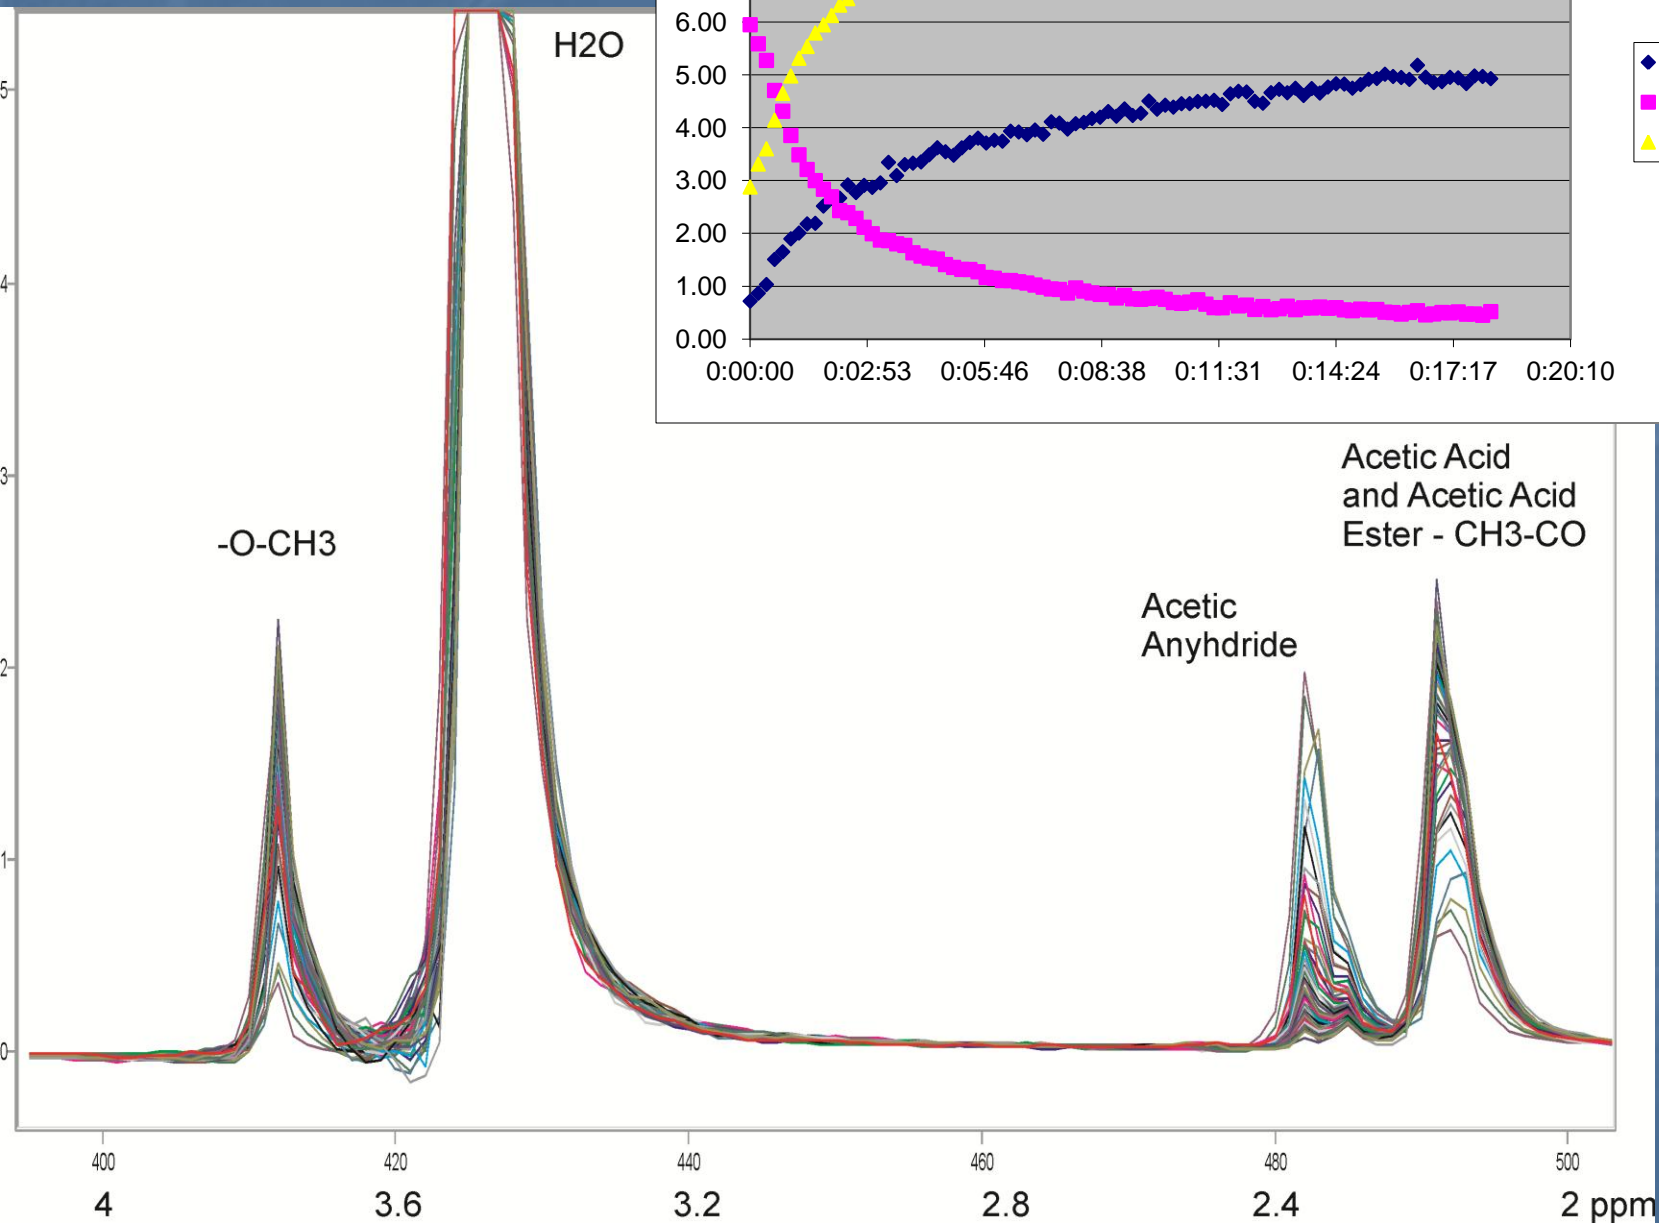










Acetic Anhydride + Methanol  
Acid Catalyzed  
No Shaking


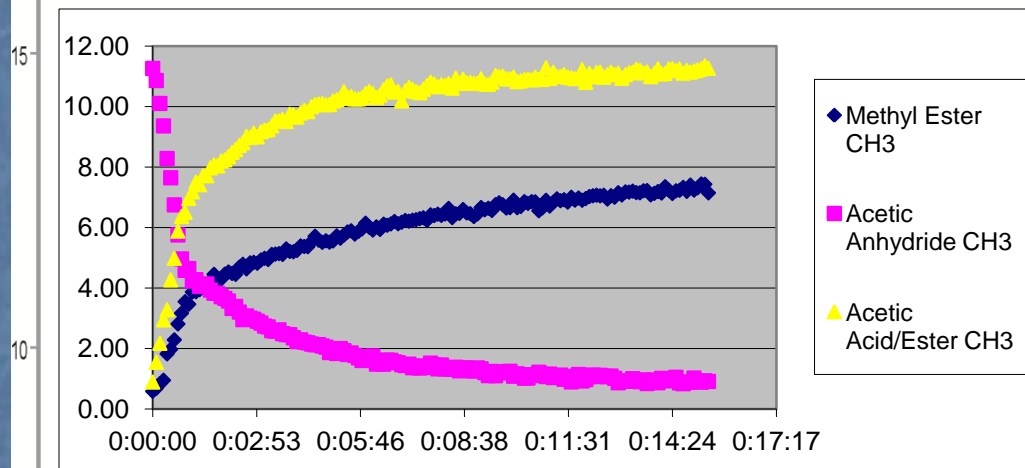


Methanol

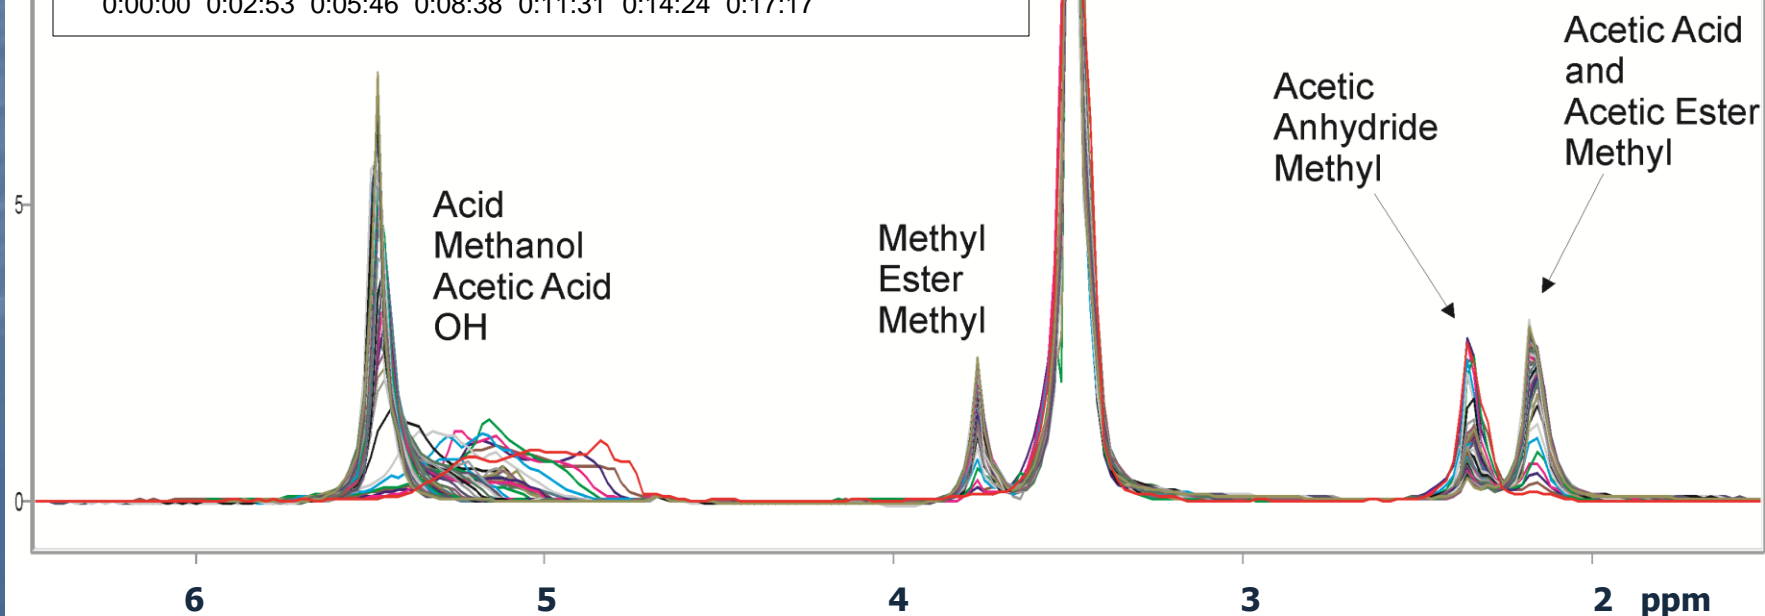

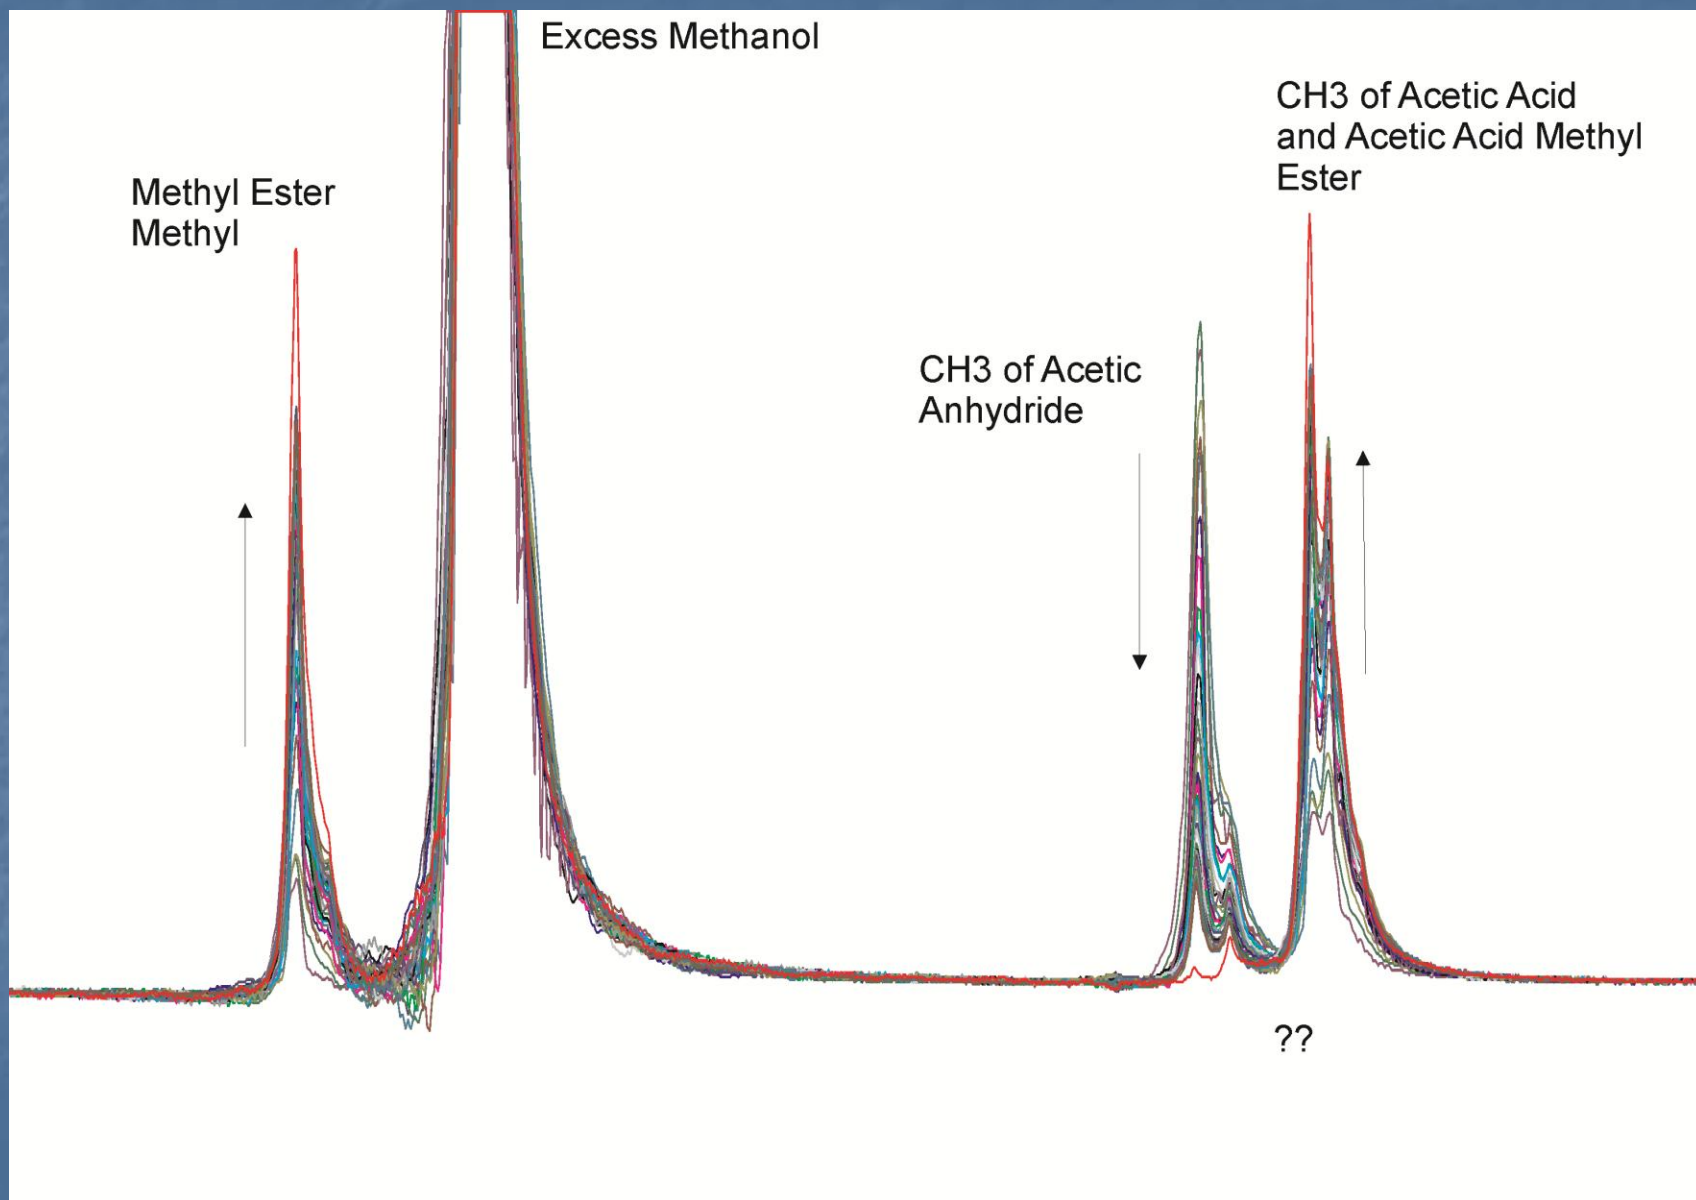

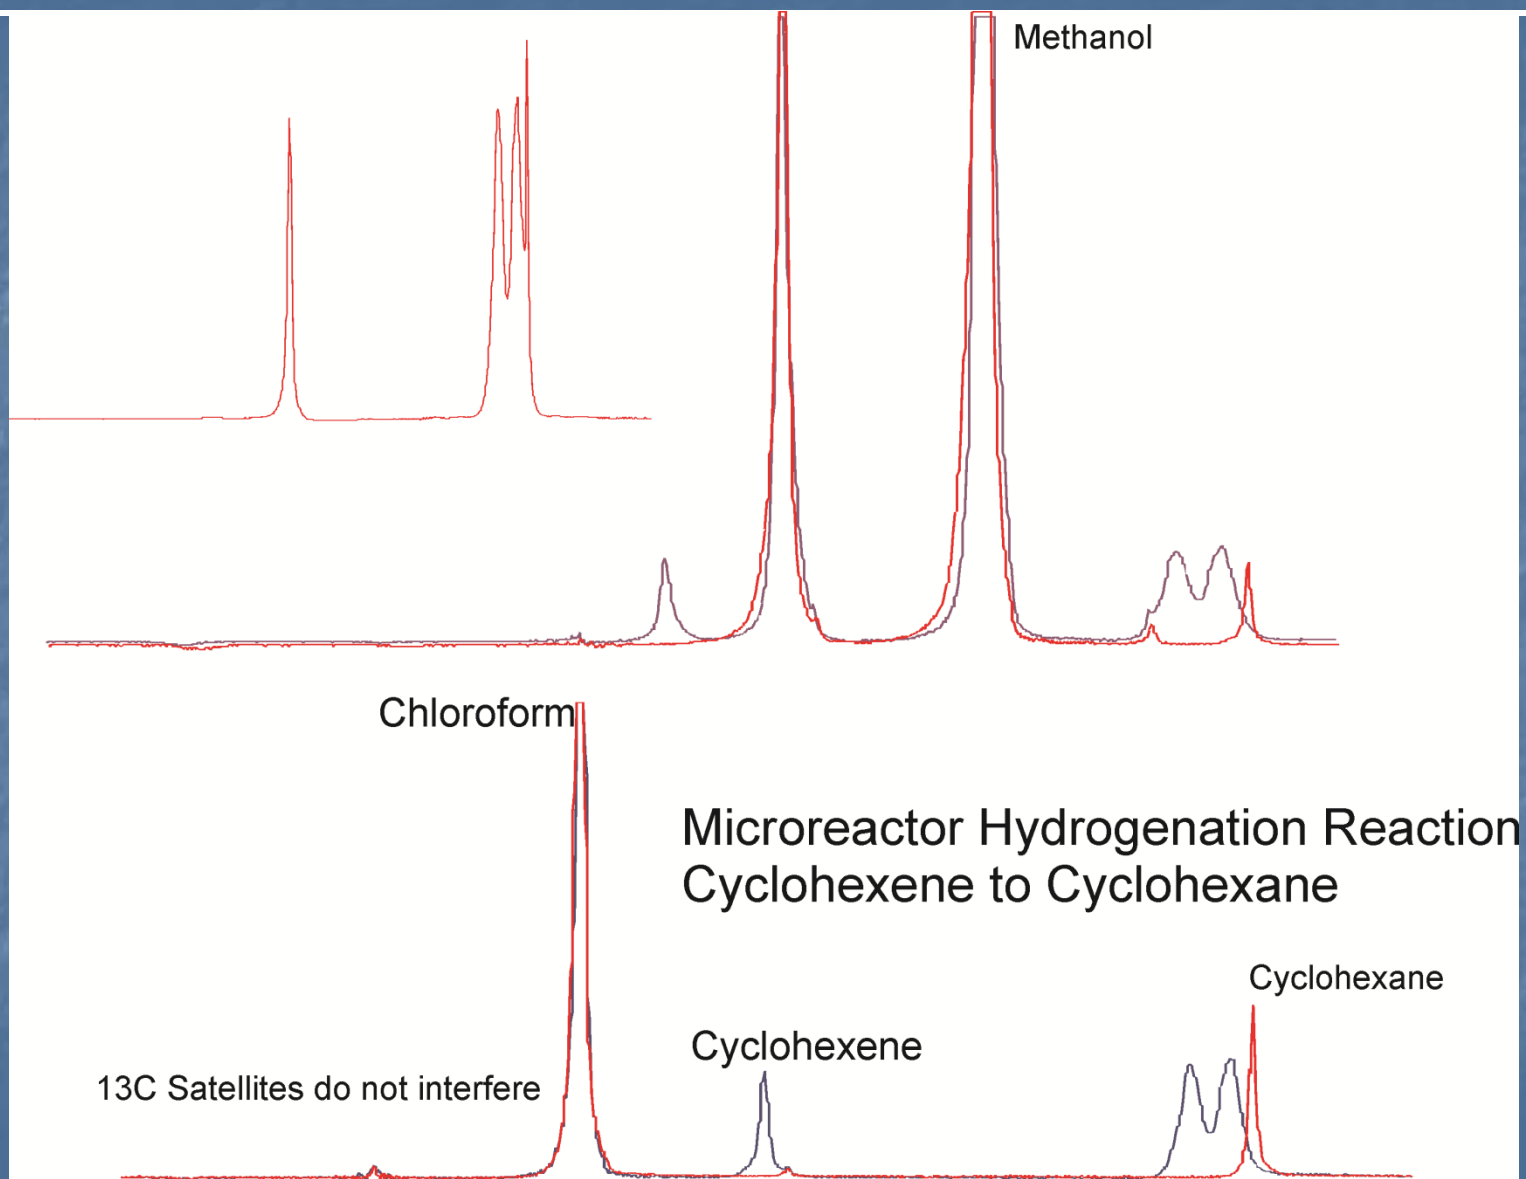

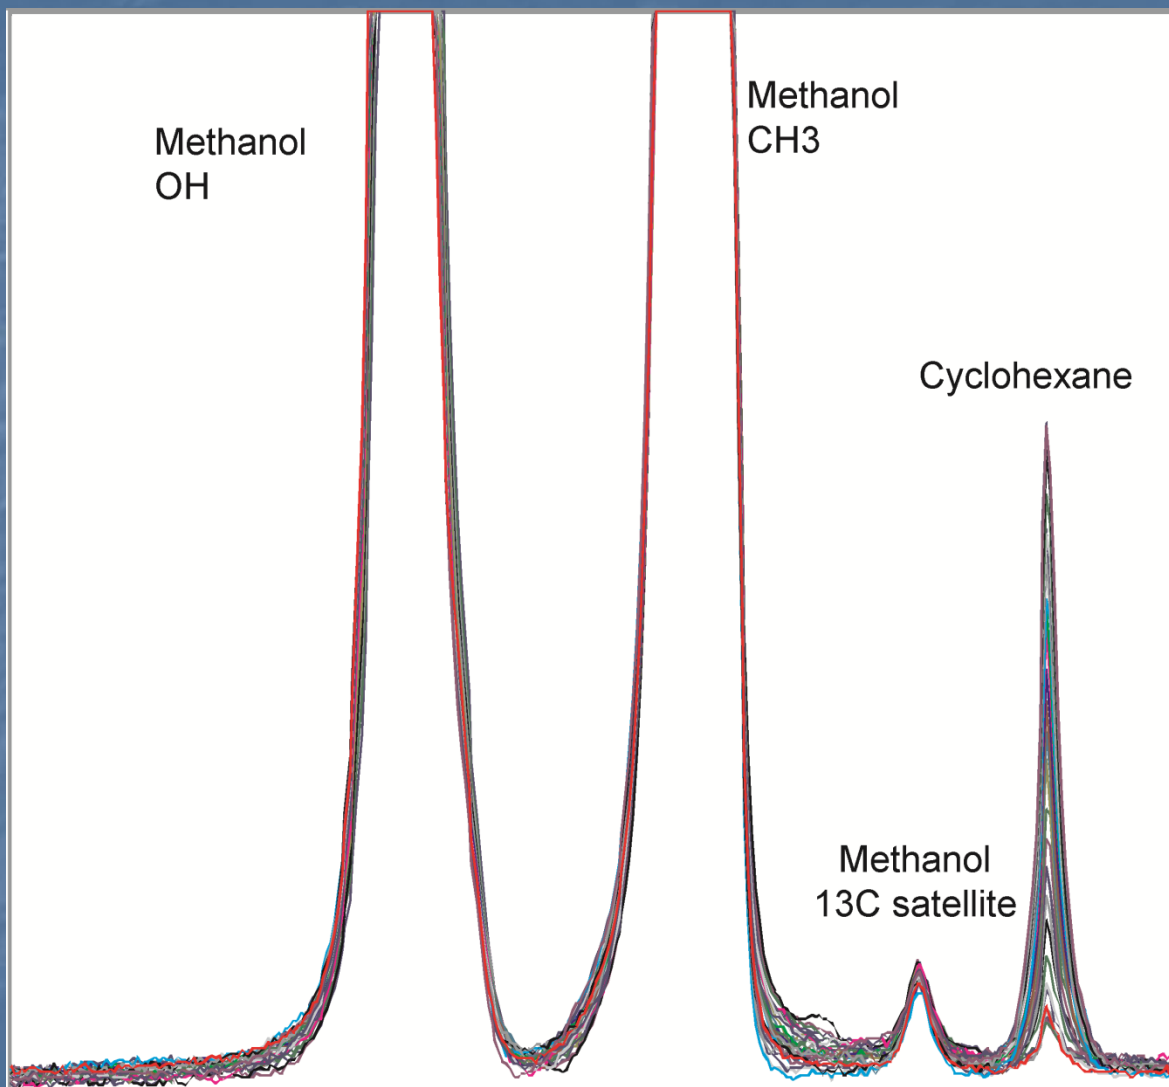

Continuous Flow (10 ml/min).  
Starting Cyclohexane concentration 0.08 gm/18 ml MeOH.  
Final Cyclohexane concentration 0.4 gm in 18 ml MeOH.  
Cyclohexane was added in 0.01 gm increments every 12 seconds with no mixing.  
Total run time: 9 minutes.